

Sample Name :PACAP (6-38), human, ovine, rat
 Cat No. :RP10338
 Lot No. :E4700119I
 Time Processed :15:25:38
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	65
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	0
40.00	Pumps	Pump A B.Conc	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

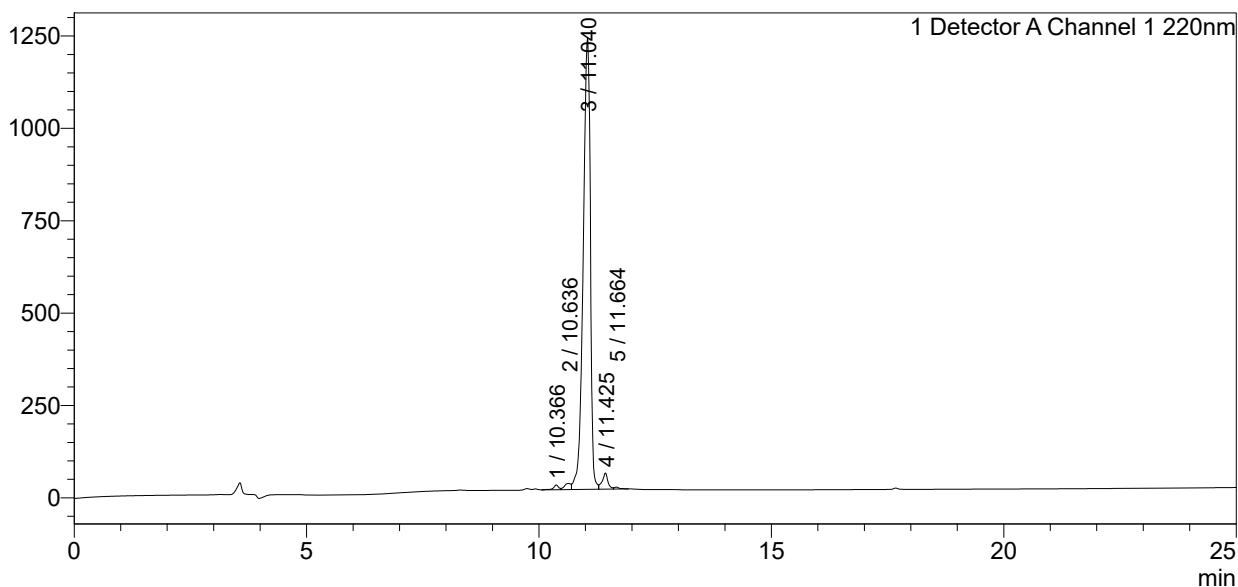

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.366	95947	12986	0.698
2	10.636	164219	16284	1.195
3	11.040	13071128	1220178	95.113
4	11.425	371395	43596	2.702
5	11.664	40117	5331	0.292
Total		13742806	1298376	100.000