


# Mass Spectrum

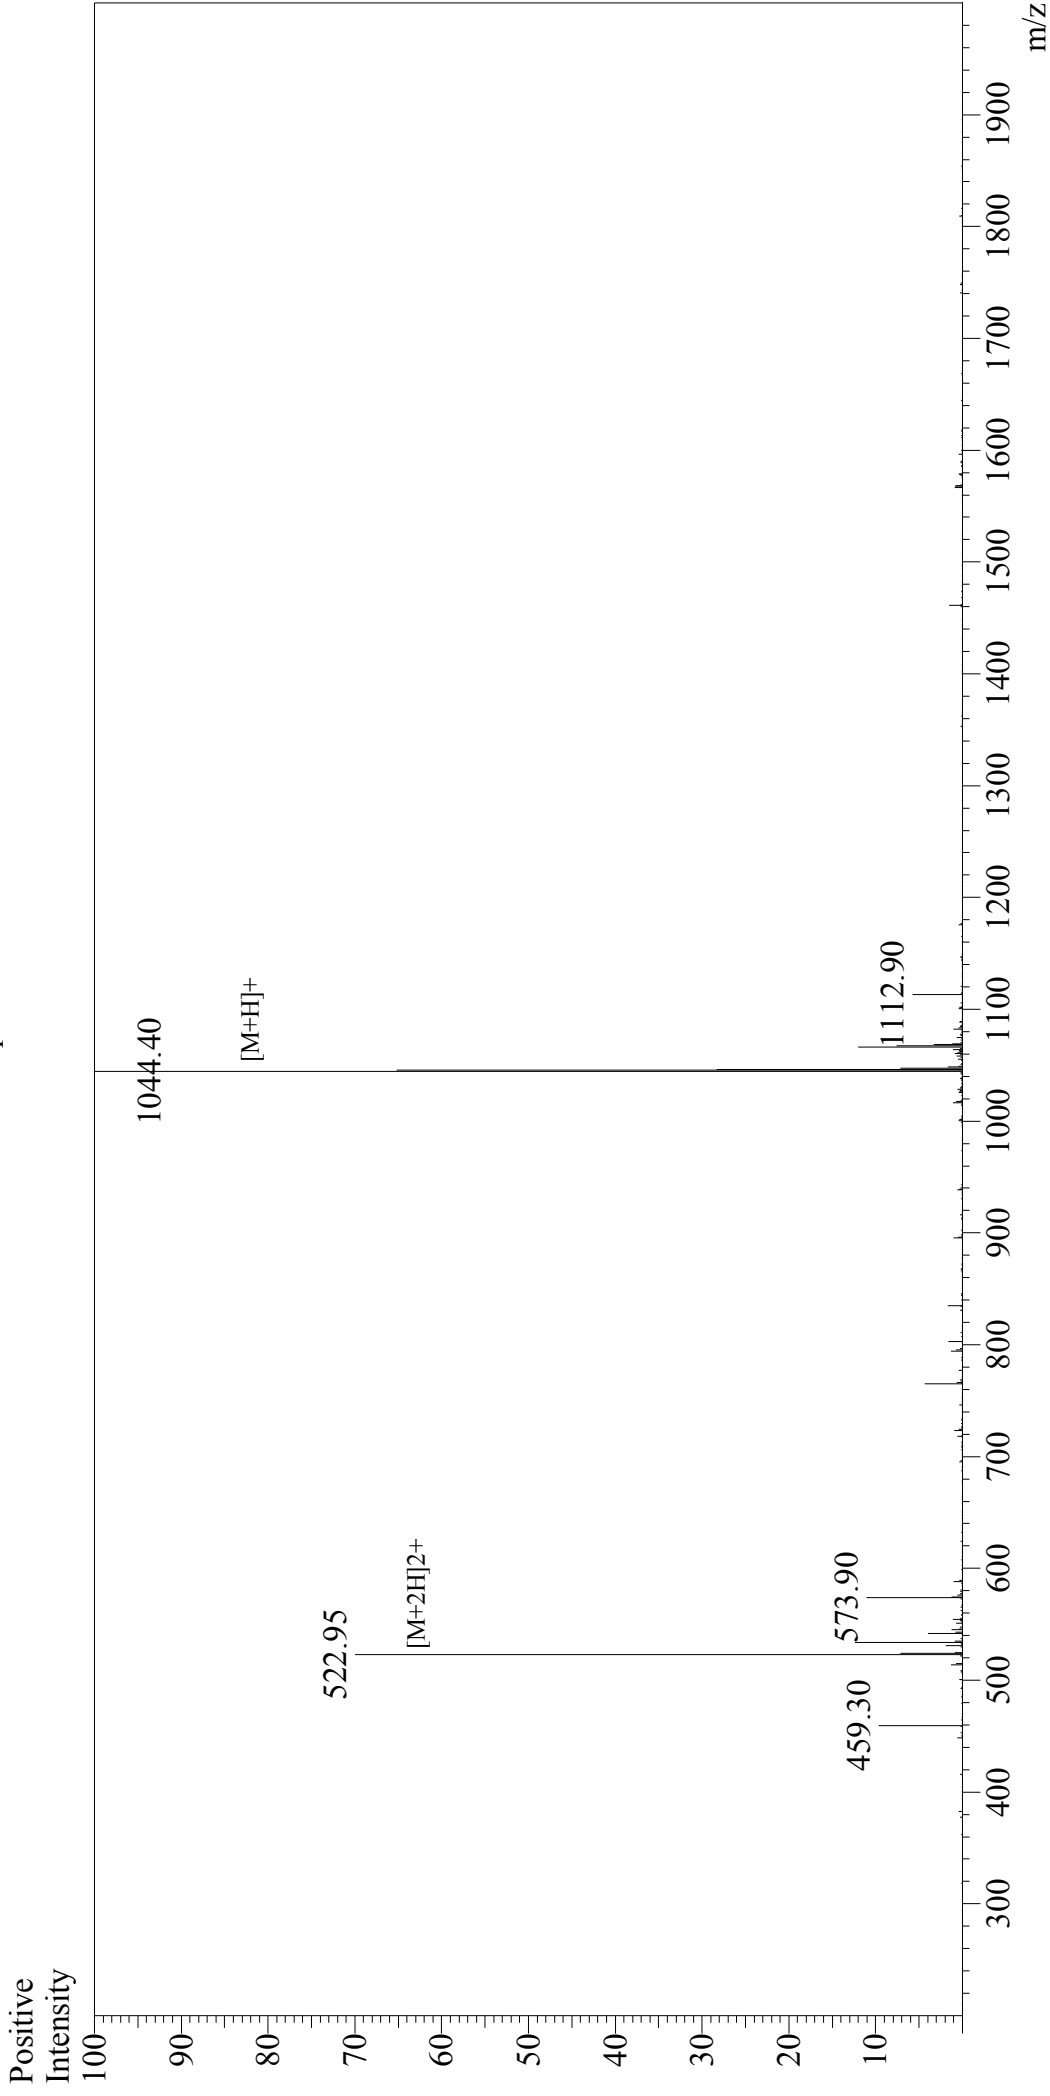

## Sample Information

User : Gary  
Month-Day Processed : 07/26/16  
Time Processed : 10:47:16  
Injection Volume : 0.2  
Sample Name : LCMV\_gp33-41  
Cat No. : RP20257  
Lot No. : PE2241705  
Theoretical MW : 1044.25  
Observed MW : 1043.40

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250°C  
Block Temp : 200°C

Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH