

Sample Name :Somatostatin

Cat. No. : RP10226 Lot. No. : PE3081807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

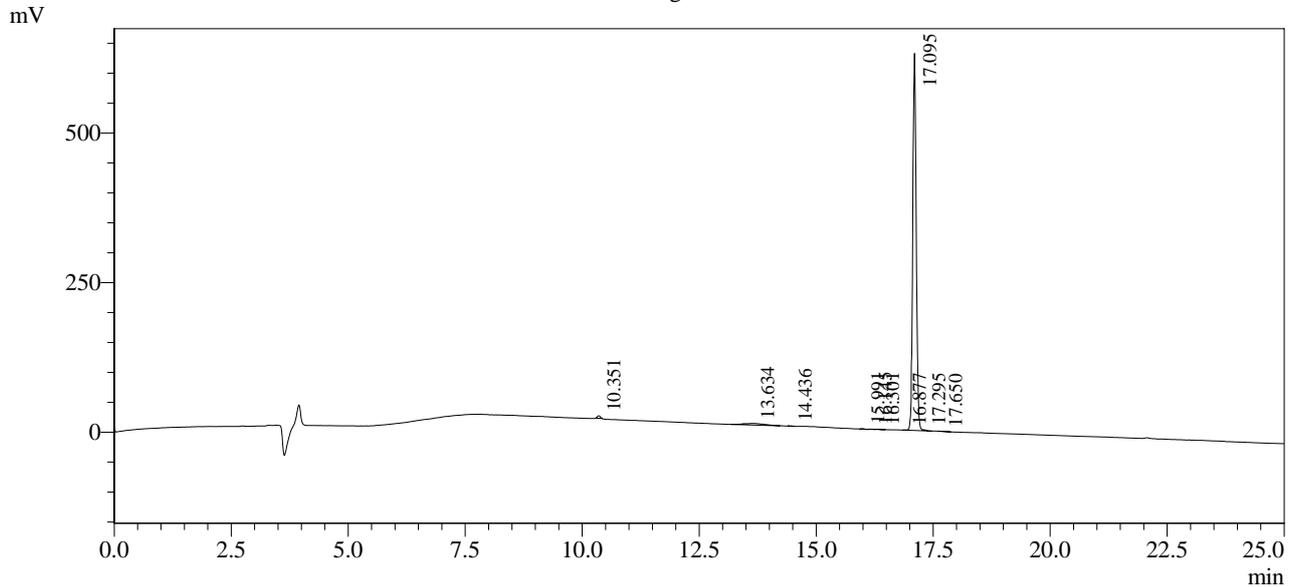

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.351	17281	4123	0.508
2	13.634	86059	2702	2.531
3	14.436	1135	265	0.033
4	15.991	2644	646	0.078
5	16.145	1813	365	0.053
6	16.301	2695	624	0.079
7	16.877	1137	354	0.033
8	17.095	3275757	630149	96.340
9	17.295	7359	1788	0.216
10	17.650	4324	485	0.127
Total		3400202	641501	100.000