

Sample Name:SAMs Peptide
 Cat No. : RP10172
 Lot No. : E1582721G
 Time Processed : 3:06:37
 Month-Day-Year Processed : 07/13/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

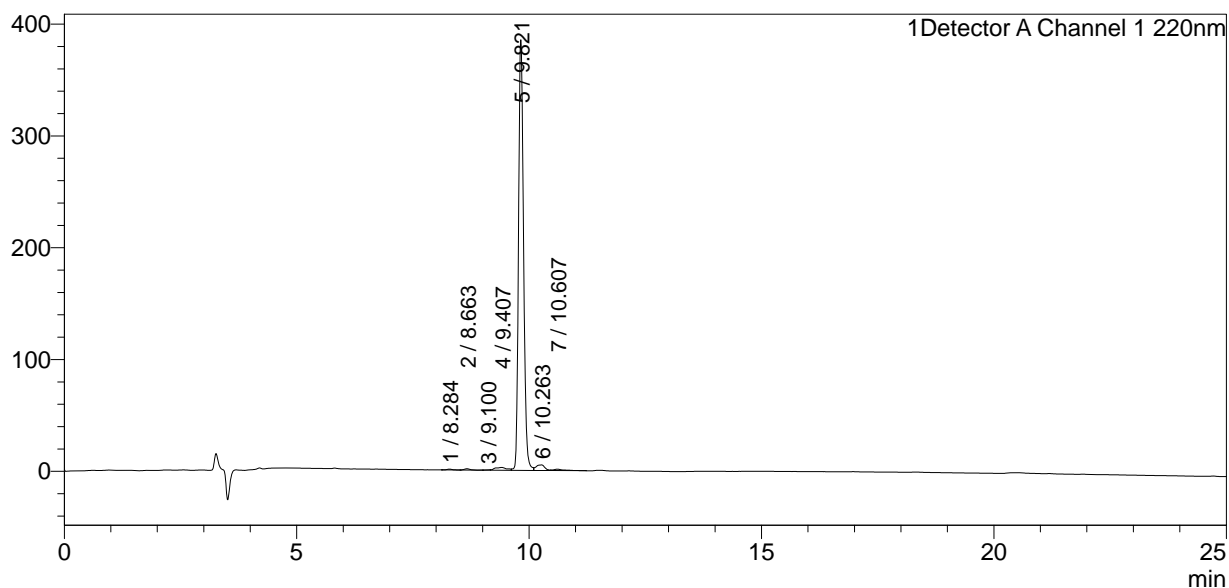

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.284	5501	739	0.182
2	8.663	10160	1174	0.336
3	9.100	2085	294	0.069
4	9.407	44422	2524	1.470
5	9.821	2875342	379977	95.144
6	10.263	64853	4969	2.146
7	10.607	19738	1221	0.653
Total		3022101	390897	100.000