


Mass Spectrum

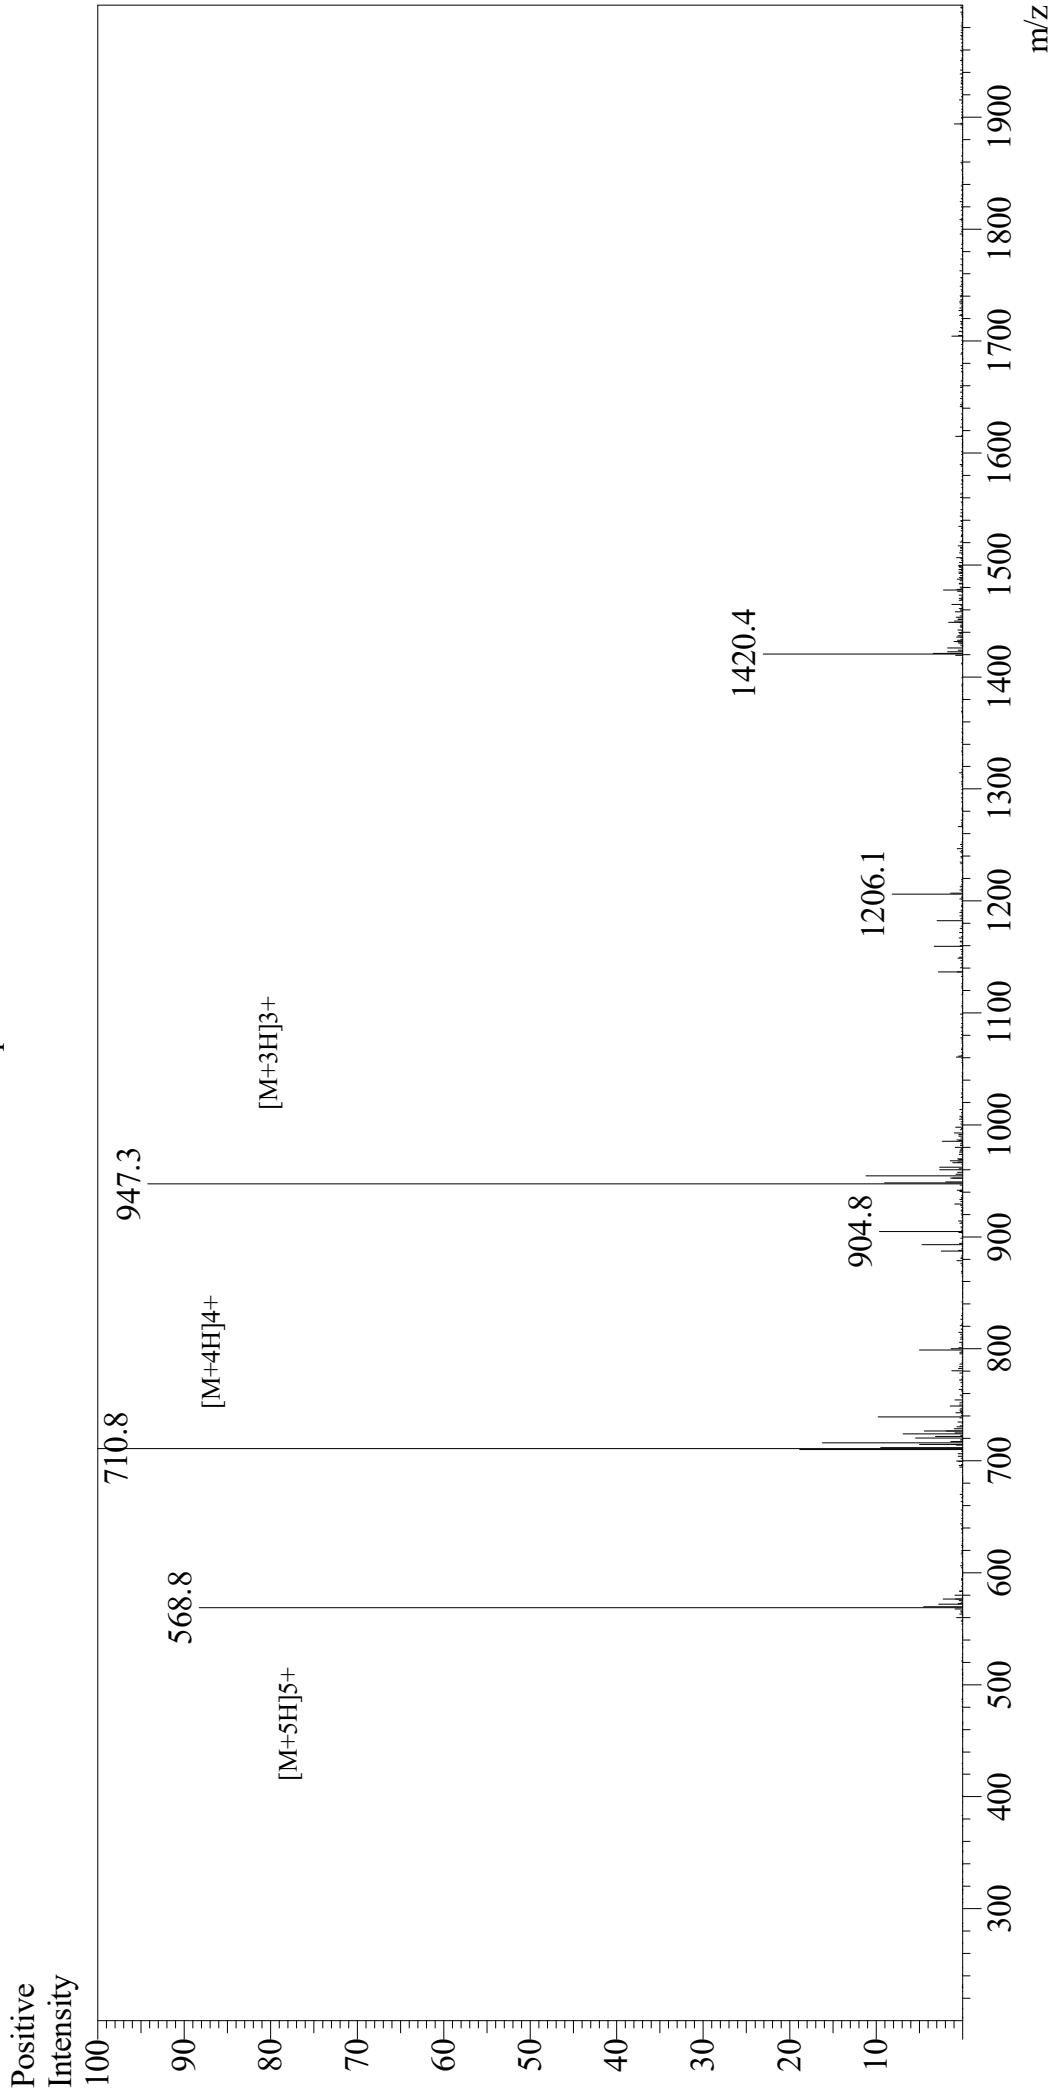

Sample Information

User : Gary
Month-Day Processed : 12/13/18
Time Processed : 10:29:58 AM
Injection Volume : 0.1
Sample Name : BAM-22P
Cat No. : RP10424
Lot No. : PE5941812
Theoretical MW : 2839.23
Observed MW : 2839.2

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH