

Sample Name : HER2/neu (654-662) GP2  
 Cat. No. : RP17314  
 Lot. No. : E4901119I  
 Time Processed : 16:01:42  
 Month-Day-Year Processed : 09/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	25	
25.00	Pumps	Pump A B.Conc	85	
31.00	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	25	
40.00	Pumps	Pump A B.Conc	25	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

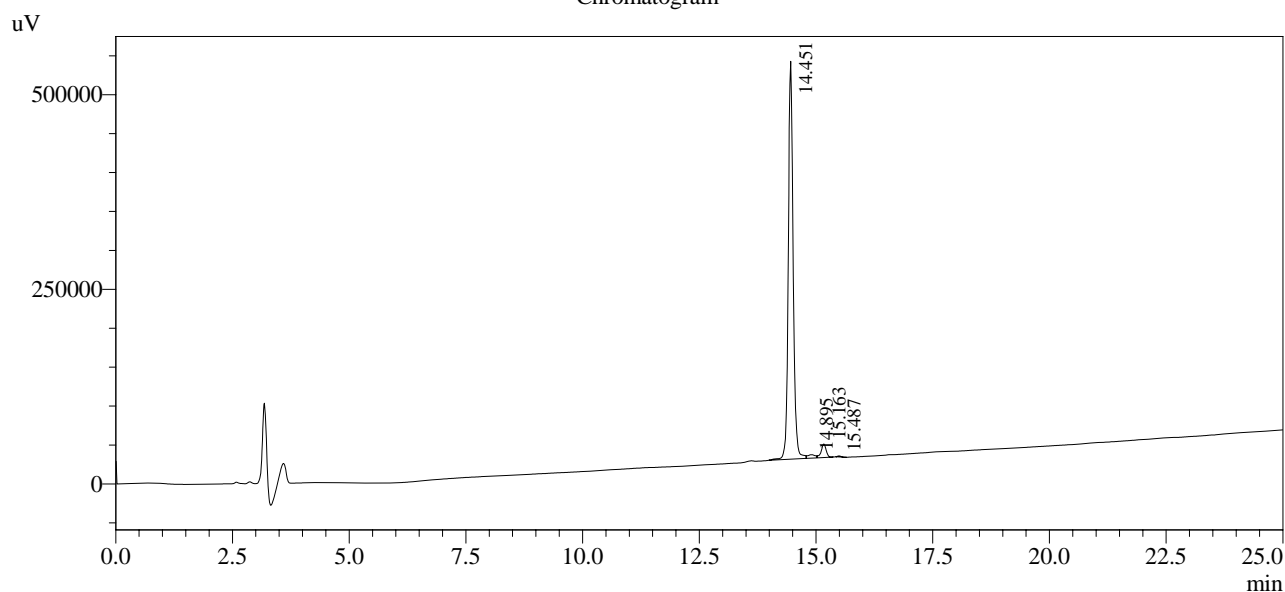

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.451	3695745	511147	95.325
2	14.895	49455	4426	1.276
3	15.163	125797	17282	3.245
4	15.487	6015	1255	0.155
Total		3877012	534111	100.000