

Sample Name: CREBtide
 Cat. No. : RP10142
 Lot. No. : E6167019I
 Time Processed: 8:14:25 AM
 Month-Day-Year

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

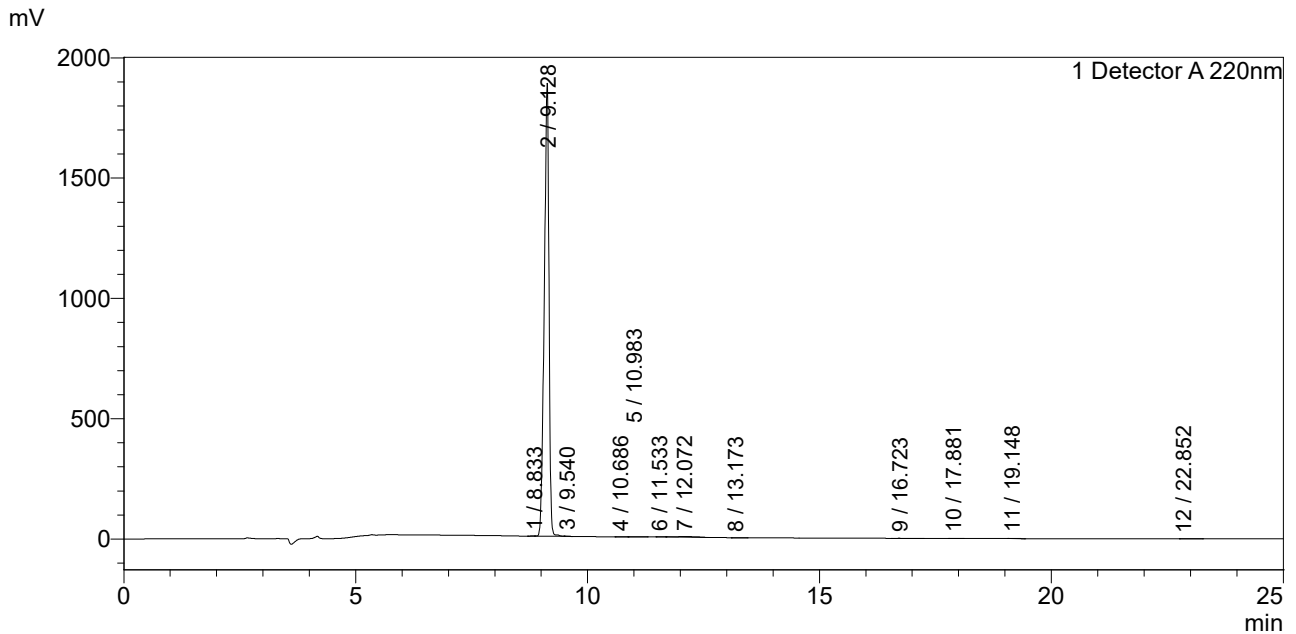

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.833	4458	690	0.034
2	9.128	13184565	1882937	99.180
3	9.540	1616	321	0.012
4	10.686	1788	235	0.013
5	10.983	4720	618	0.036
6	11.533	1011	129	0.008
7	12.072	85573	2554	0.644
8	13.173	1634	101	0.012
9	16.723	4220	170	0.032
10	17.881	1572	166	0.012
11	19.148	1114	78	0.008
12	22.852	1365	84	0.010
Total		13293637	1888084	100.000