

Sample Name :β-MSH, human
 Lot No. :RP10648
 Cat No. :PE5881903

Time Processed : 13:52:13
 Month-Day-Year Processed : 03/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

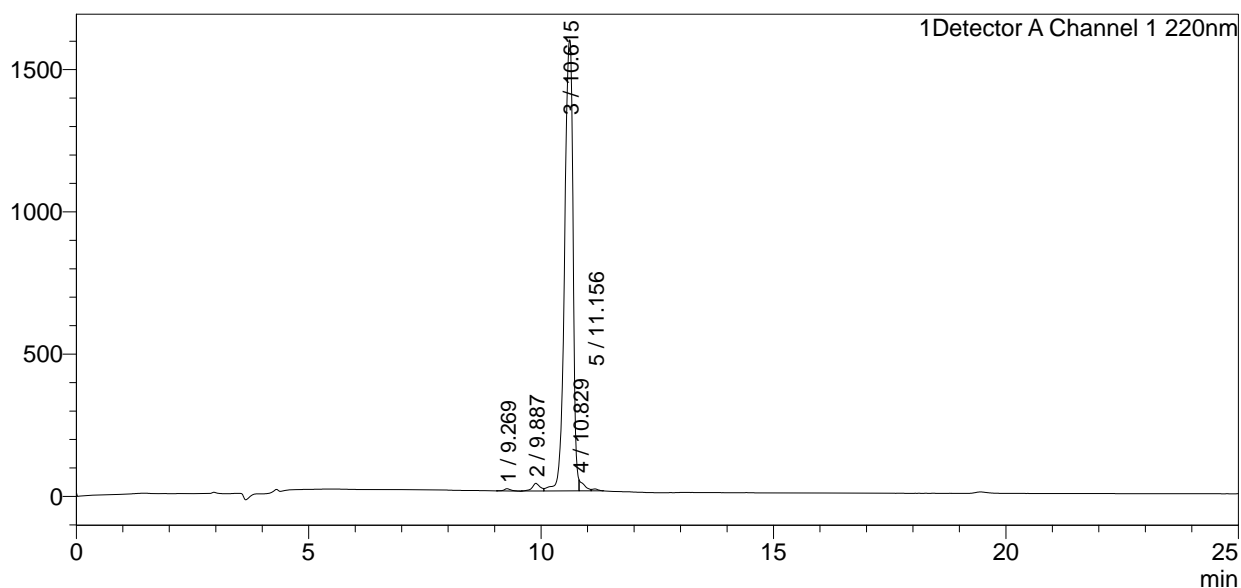

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.269	79089	8024	0.383
2	9.887	317037	26877	1.536
3	10.615	19918215	1585247	96.507
4	10.829	269433	35352	1.305
5	11.156	55349	6491	0.268
Total		20639122	1661992	100.000