

Sample Name :GnRH-I
 Cat. No. :RP20303
 Lot. No. :E4666519I
 Time Processed :14:19:16
 Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

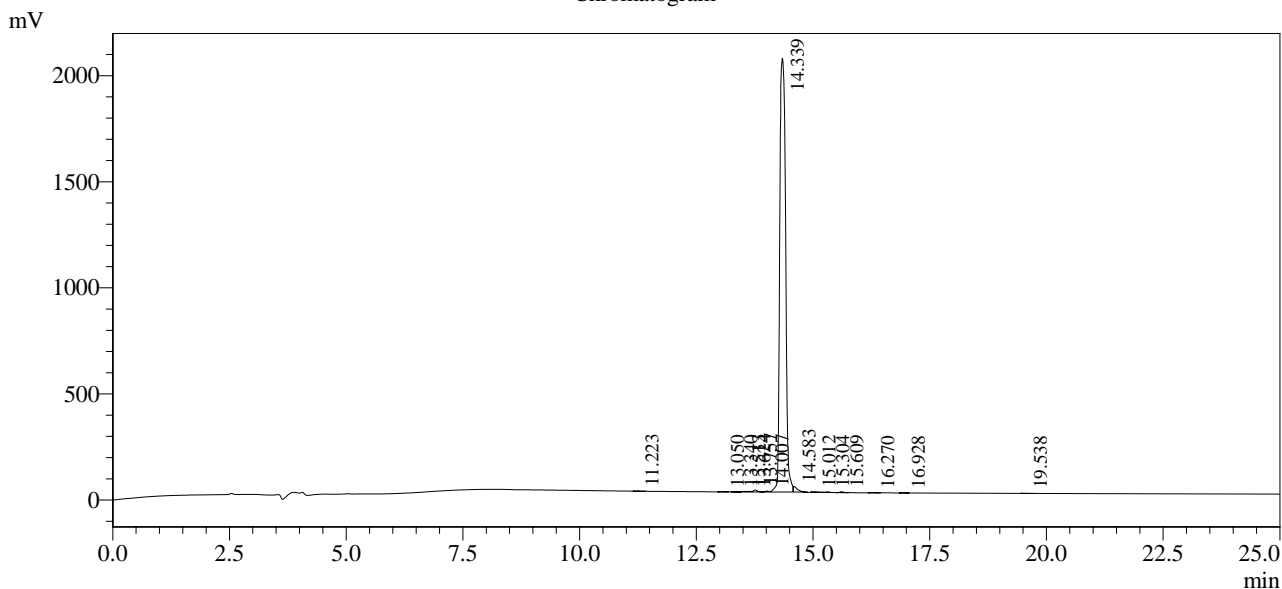

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.223	3740	586	0.021
2	13.050	8062	1532	0.045
3	13.340	7328	1458	0.040
4	13.513	17011	3008	0.094
5	13.624	20038	3305	0.111
6	13.757	58892	9564	0.325
7	14.007	26835	4389	0.148
8	14.339	17751259	2044566	98.044
9	14.583	158155	26873	0.874
10	15.012	8184	952	0.045
11	15.304	14745	2764	0.081
12	15.609	21723	3985	0.120
13	16.270	3892	714	0.021
14	16.928	2133	376	0.012
15	19.538	3472	547	0.019
Total		18105469	2104618	100.000