

Sample Name :ANP (1-28), human, porcine
 Cat. No. : RP11927
 Lot. No. : PE5901812
 Time Processed : 15:52:20
 Month-Day-Year Processed : 01/09/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

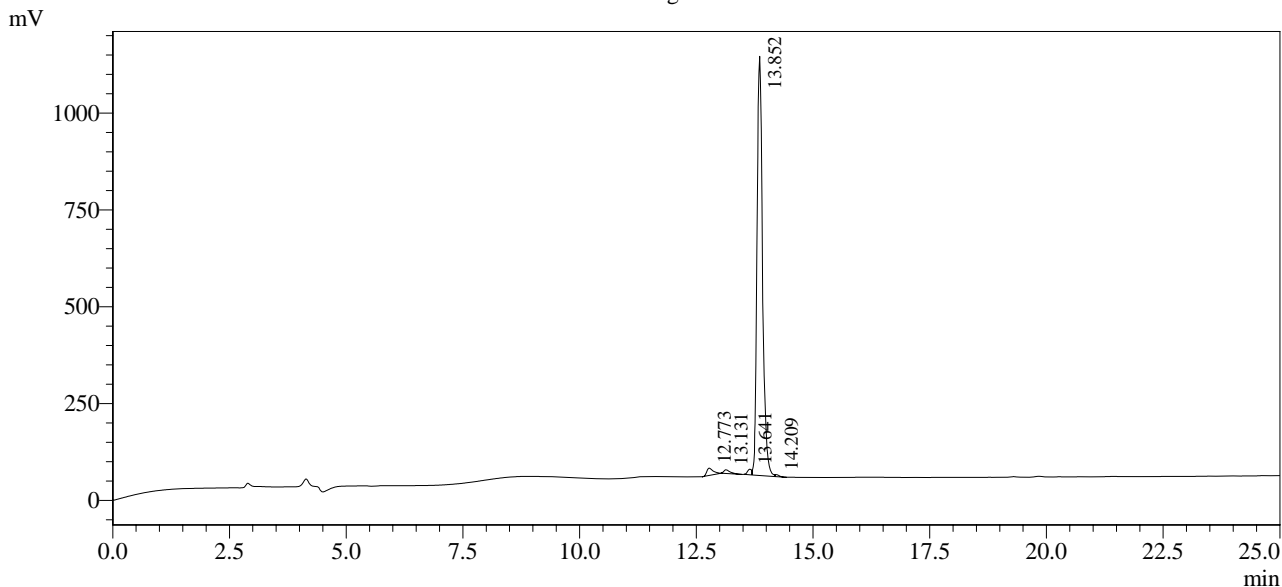

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.773	184956	18987	1.983
2	13.131	88289	9610	0.947
3	13.641	87822	14258	0.942
4	13.852	8937433	1082232	95.829
5	14.209	27965	5118	0.300
Total		9326466	1130206	100.000