

Sample Name :Neuropeptide Y,human  
 Cat No. :RP10492  
 Lot No. :PE4721903  
 Time Processed : 15:48:21  
 Month-Day-Year Processed :03/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

### <Chromatogram>

mV

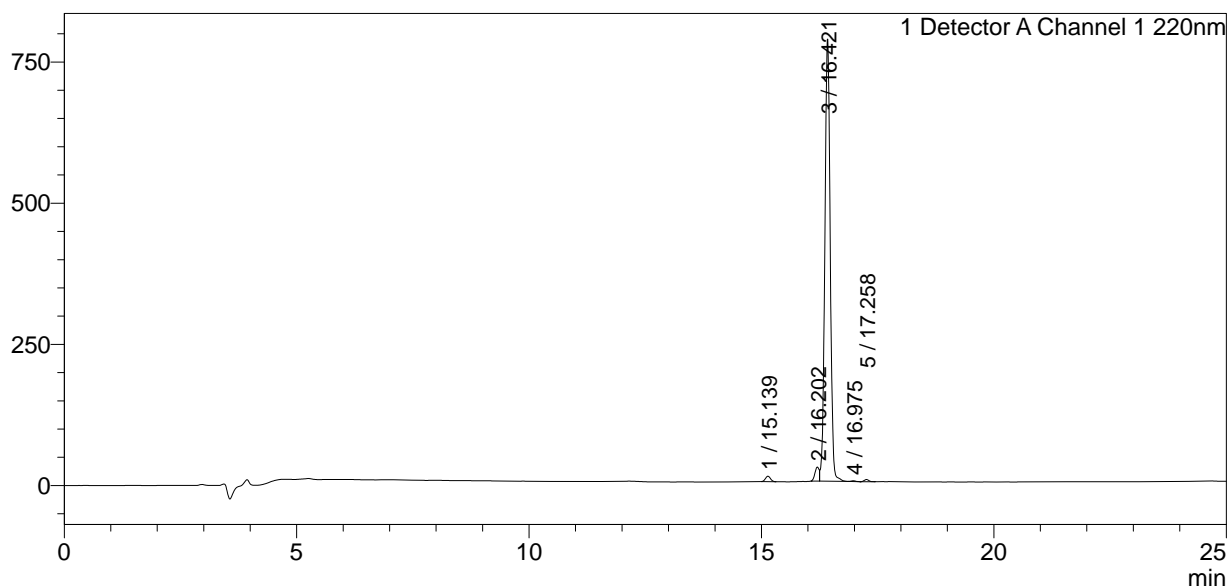

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.139	71313	9566	1.088
2	16.202	157435	24852	2.403
3	16.421	6289805	782941	95.986
4	16.975	8532	1376	0.130
5	17.258	25724	3953	0.393
Total		6552808	822688	100.000