

Sample Name :GRGDSP
 Cat No. :RP20255
 Lot No. :E4850419I
 Time Processed :7:32:58
 Month-Day-Year Processed :09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

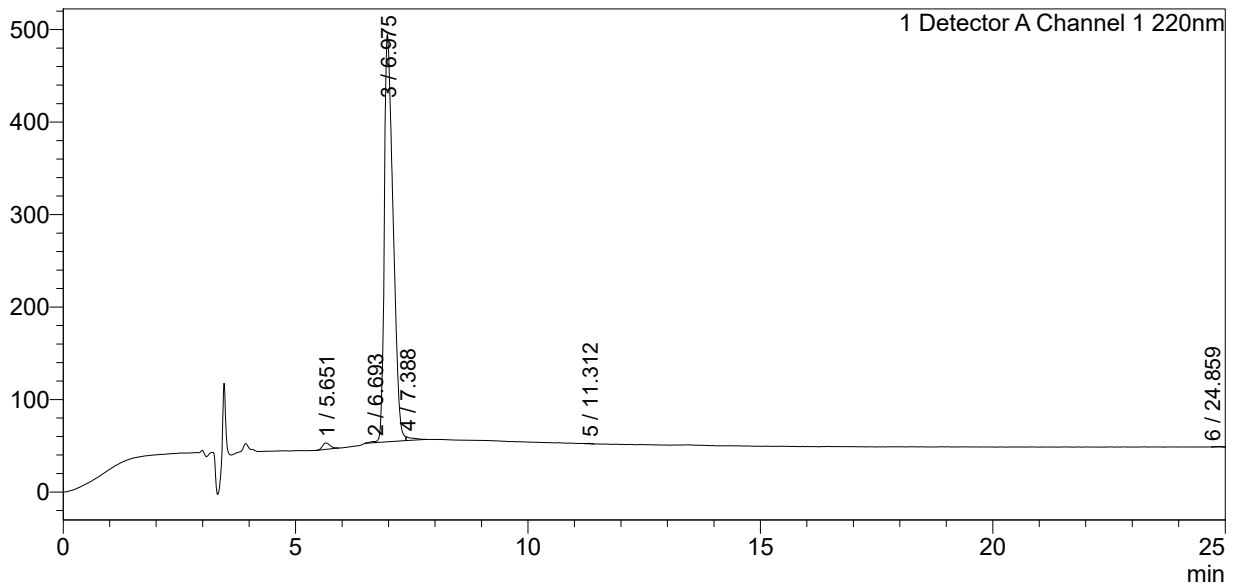

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.651	76662	6865	1.301
2	6.693	11110	1281	0.188
3	6.975	5758815	440343	97.700
4	7.388	41310	4017	0.701
5	11.312	1891	440	0.032
6	24.859	4622	516	0.078
Total		5894411	453462	100.000