

Sample Name : β -amyloid (11-22)
 Cat No. :RP20102
 Lot No. :PE4281811
 Time Processed : 22:29:17
 Month-Day-Year Processed : 11/12/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

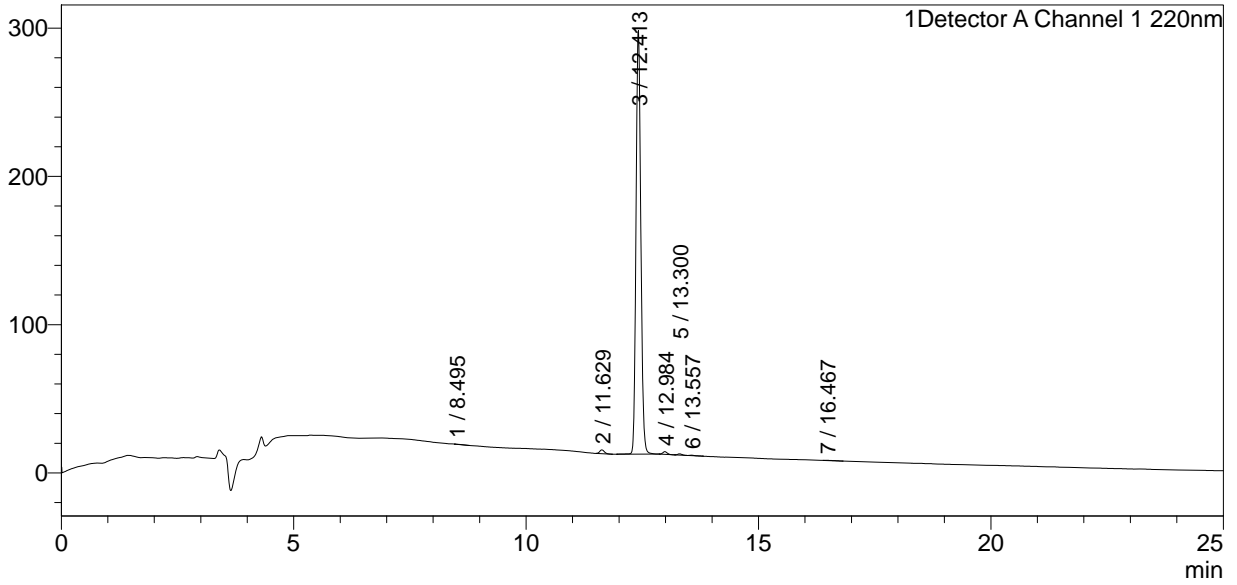

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.495	1619	122	0.077
2	11.629	17579	2575	0.838
3	12.413	2056670	285699	98.081
4	12.984	11846	1828	0.565
5	13.300	5315	844	0.253
6	13.557	1883	290	0.090
7	16.467	1995	177	0.095
Total		2096906	291536	100.000