

Sample Name: Ia52
 Cat No. : RP20228
 Lot No. : E2090620F
 Time Processed: 12:56:21 PM
 Month-Day-Year Processed :07/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

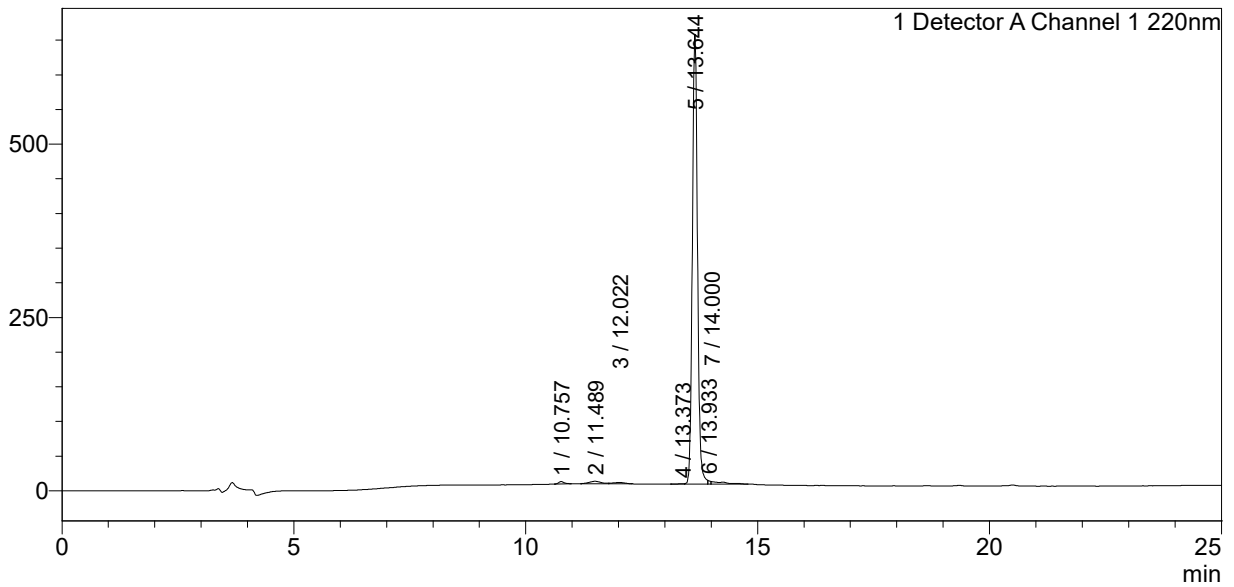

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.757	29159	3565	0.557
2	11.489	63561	3532	1.215
3	12.022	34758	1912	0.665
4	13.373	8401	830	0.161
5	13.644	4999327	649209	95.578
6	13.933	17900	5177	0.342
7	14.000	77533	3803	1.482
Total		5230639	668029	100.000