


# Mass Spectrum

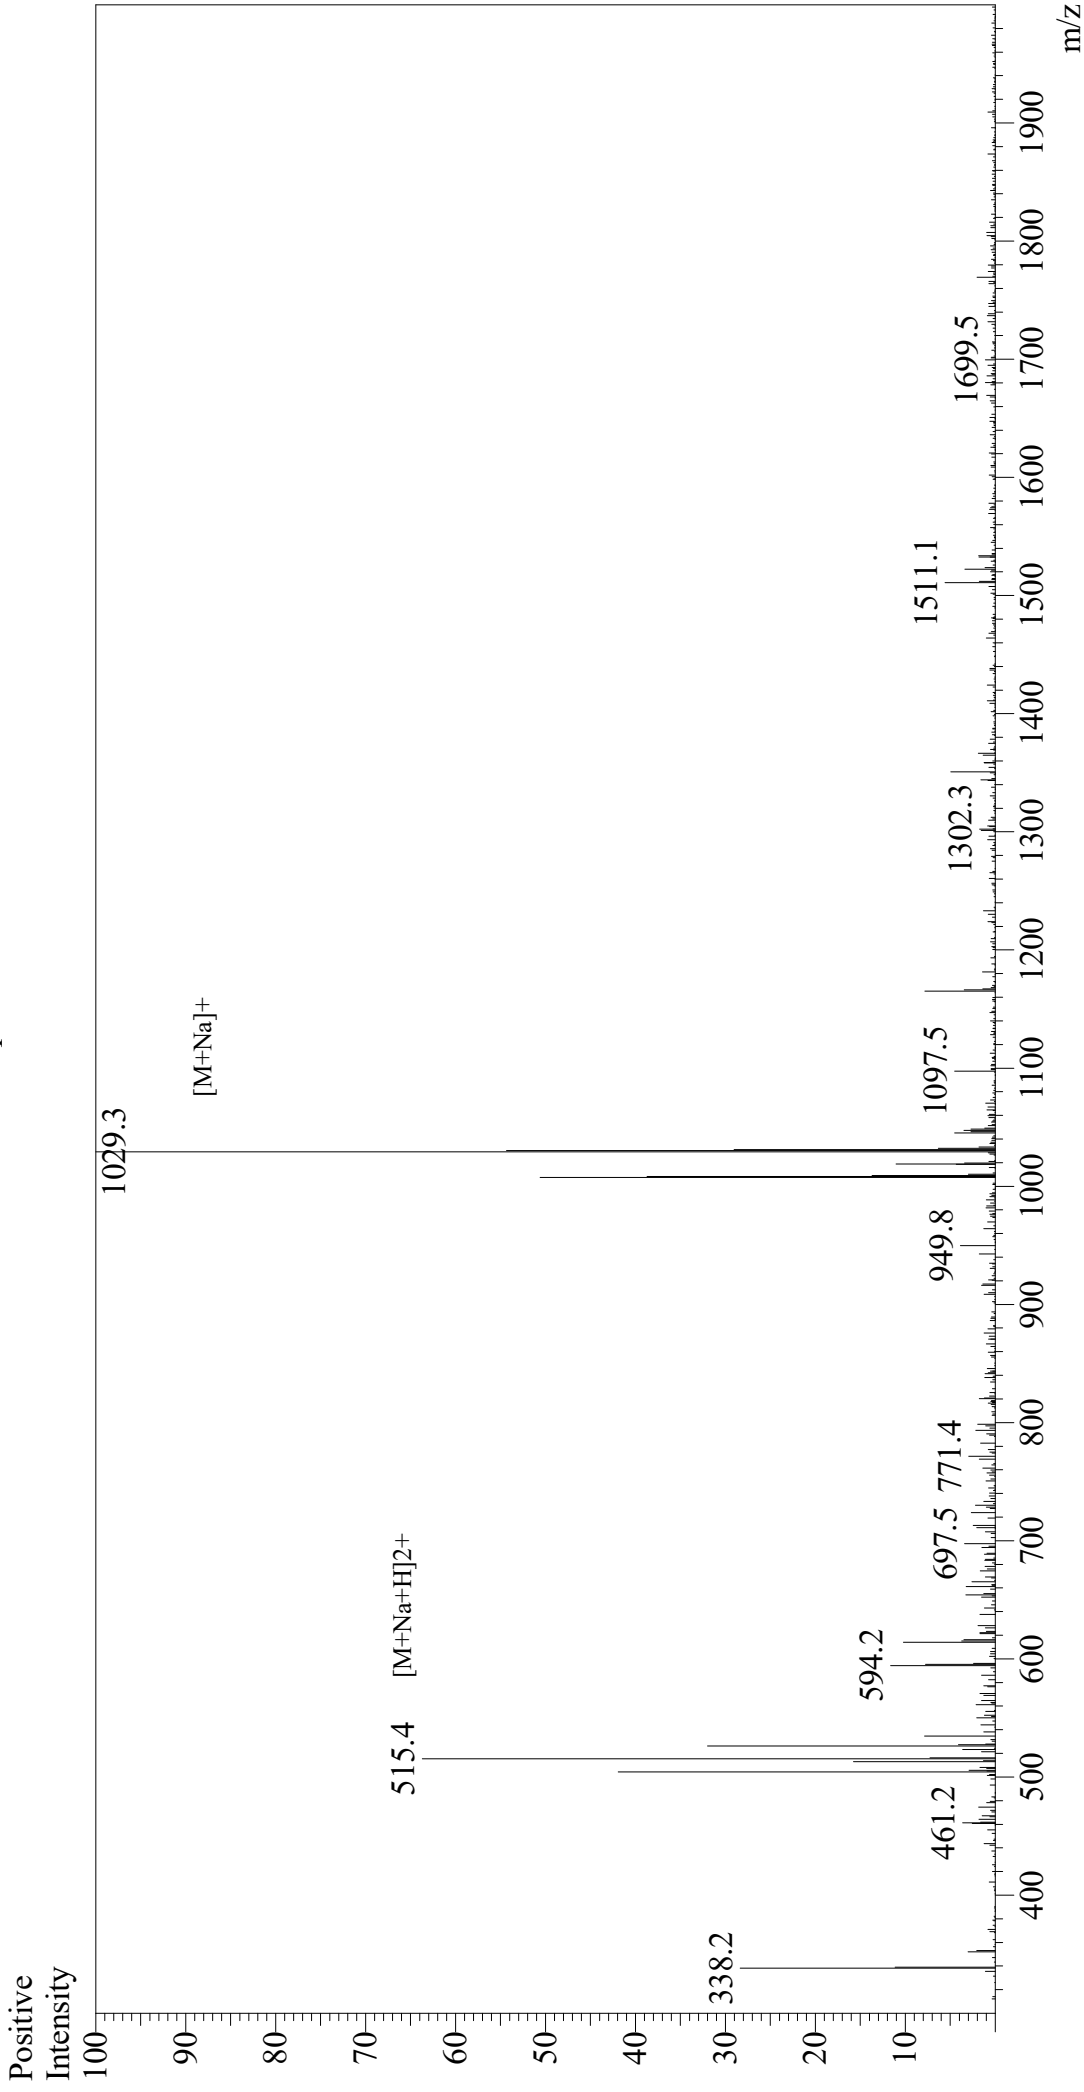

Sample Information  
 Month-Day Processed : 11/18/20  
 Time Processed : 11:47:05 AM  
 Injection Volume : 0.3  
 Sample Name : Oxytocin  
 Cat No. : RP10407  
 Lot No. : E4699520K  
 Theoretical MW : 1007.20  
 Observed MW : 1007.3

Interface : ESI  
 Nebulizing Gas Flow : 1.5L/min  
 CDL Temp : 250  
 Block Temp : 200

Equipment : GK11010007  
 Interface Bias : +4.5 kV  
 Drying Gas Flow : 5 L/min  
 T.Flow : 0.2 ml/min  
 B.conc : 50%H2O/50%MeOH