

Sample Name : YRGDS Fibronectin Fragment  
 Cat No.: RP20476  
 Lot No.: E4982919I  
 Time Processed: 7:08:15  
 Month-Day-Year Processed: 09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010014

<Chromatogram>

mV

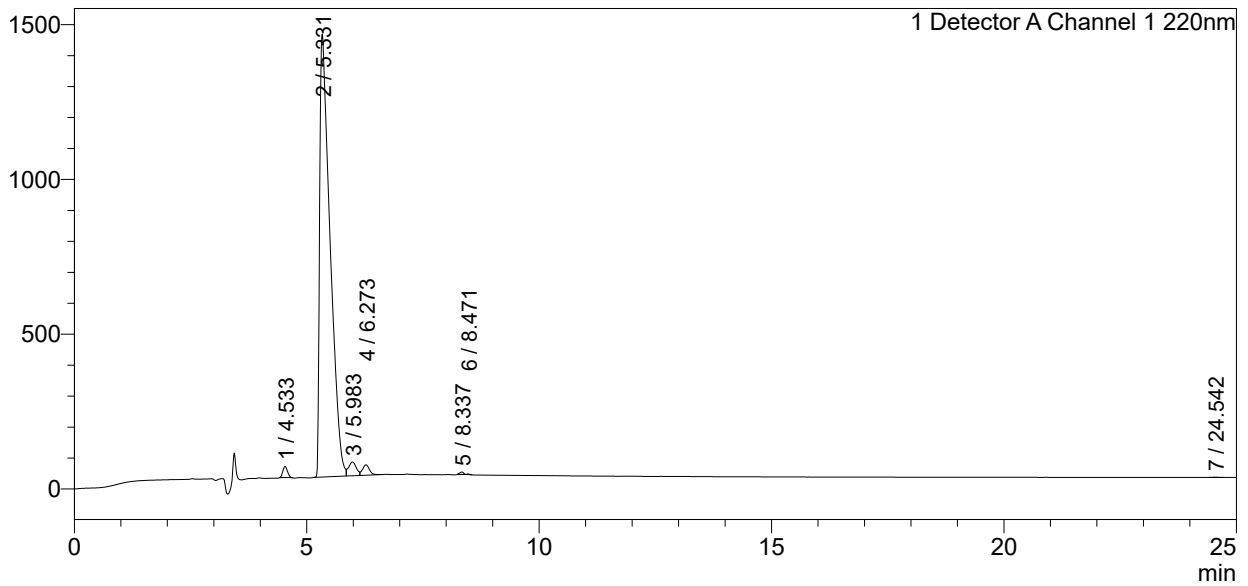

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.533	245553	35971	1.049
2	5.331	22242824	1430779	95.023
3	5.983	515879	44444	2.204
4	6.273	345281	33508	1.475
5	8.337	46699	8100	0.200
6	8.471	8386	2173	0.036
7	24.542	3234	438	0.014
Total		23407855	1555415	100.000