

Sample Name : c-Myc Peptide  
 Cat.No : RP11731  
 Lot.No : E7856120L  
 Time Processed: 14:59:05  
 Year-Month-Day: 2020/12/6

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min

<<Detector A>>  
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010015

<Chromatogram>

mV

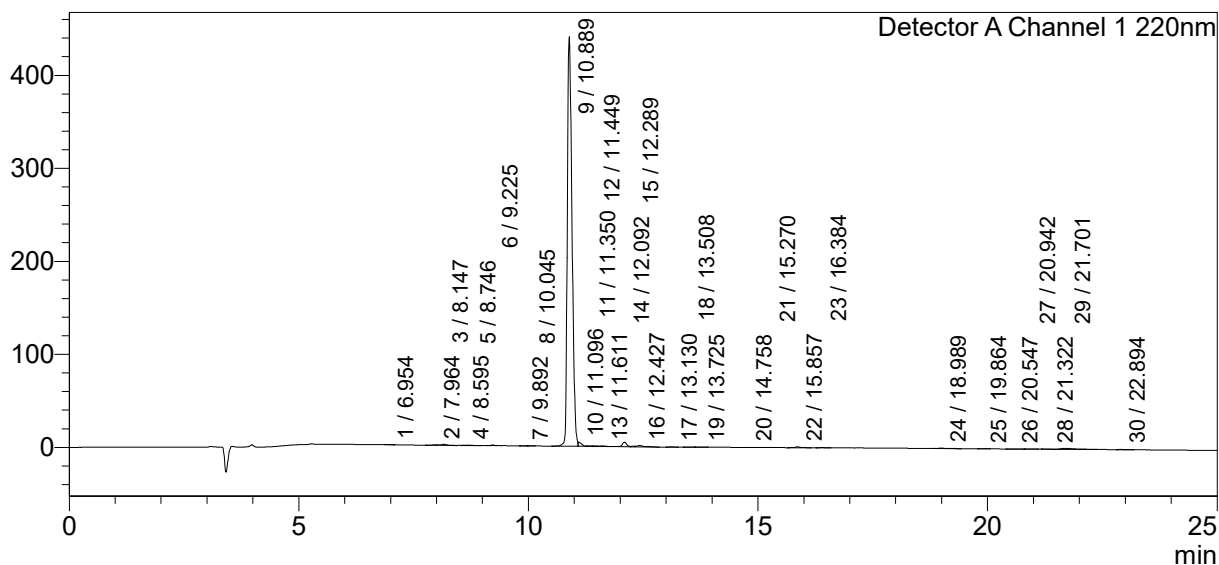

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.954	1952	302	0.060
2	7.964	2459	239	0.075
3	8.147	9650	1196	0.295
4	8.595	1174	134	0.036
5	8.746	2196	291	0.067
6	9.225	3856	699	0.118
7	9.892	1117	188	0.034
8	10.045	1011	229	0.031
9	10.889	3117166	440267	95.259
10	11.096	21713	4250	0.664
11	11.350	3676	591	0.112
12	11.449	4923	666	0.150
13	11.611	4644	621	0.142
14	12.092	30909	4831	0.945

Peak#	Ret. Time	Area	Height	Area%
15	12.289	2605	532	0.080
16	12.427	15198	1469	0.464
17	13.130	1616	219	0.049
18	13.508	1244	120	0.038
19	13.725	1154	129	0.035
20	14.758	1035	89	0.032
21	15.270	1387	162	0.042
22	15.857	7018	882	0.214
23	16.384	1690	196	0.052
24	18.989	5277	336	0.161
25	19.864	1410	138	0.043
26	20.547	1836	136	0.056
27	20.942	1032	130	0.032
28	21.322	1305	163	0.040
29	21.701	20407	897	0.624
30	22.894	1632	213	0.050
Total		3272291	460316	100.000