

Sample Name :Osteogenic Growth Peptide, OGP
 Cat. No. : RP20311
 Lot. No. : E9579319L
 Time Processed :13:34:02
 Month-Day-Year Processed : 12/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

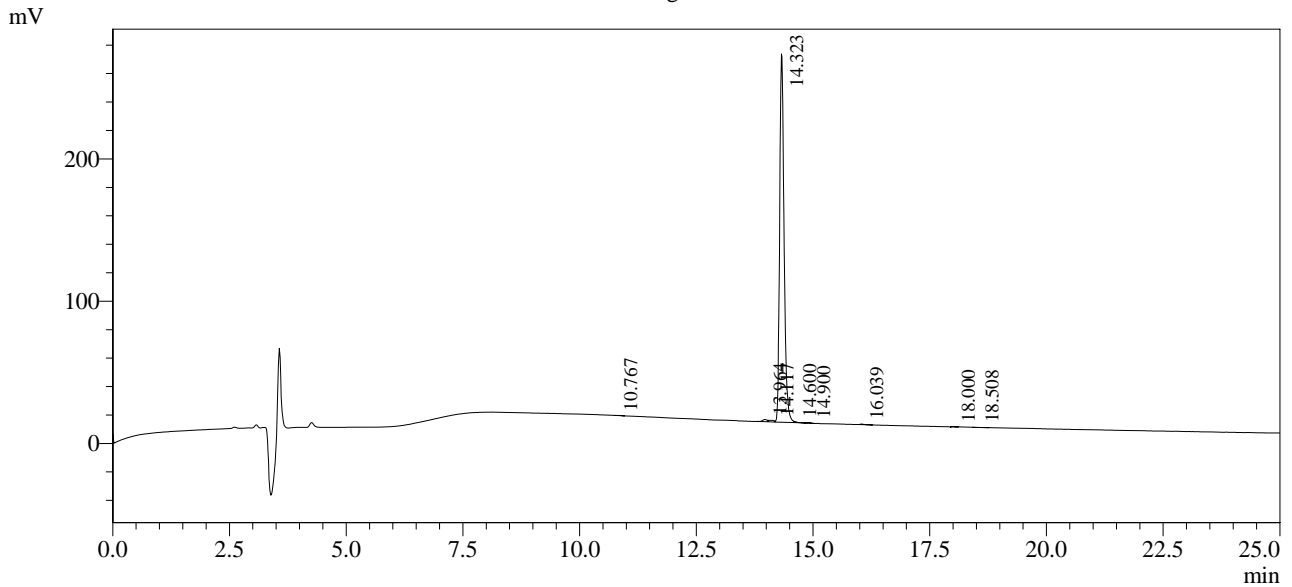

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.767	1003	57	0.058
2	13.964	11296	1549	0.652
3	14.117	8904	1157	0.514
4	14.323	1700935	258892	98.223
5	14.600	3460	898	0.200
6	14.900	1649	250	0.095
7	16.039	2168	386	0.125
8	18.000	1120	233	0.065
9	18.508	1171	125	0.068
Total		1731706	263548	100.000