

Sample Name : β -amyloid (1-11)
 Cat No. :RP20106
 Lot No. :E4830019I
 Time Processed :15:03:31
 Month-Day-Year Processed :09/20/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

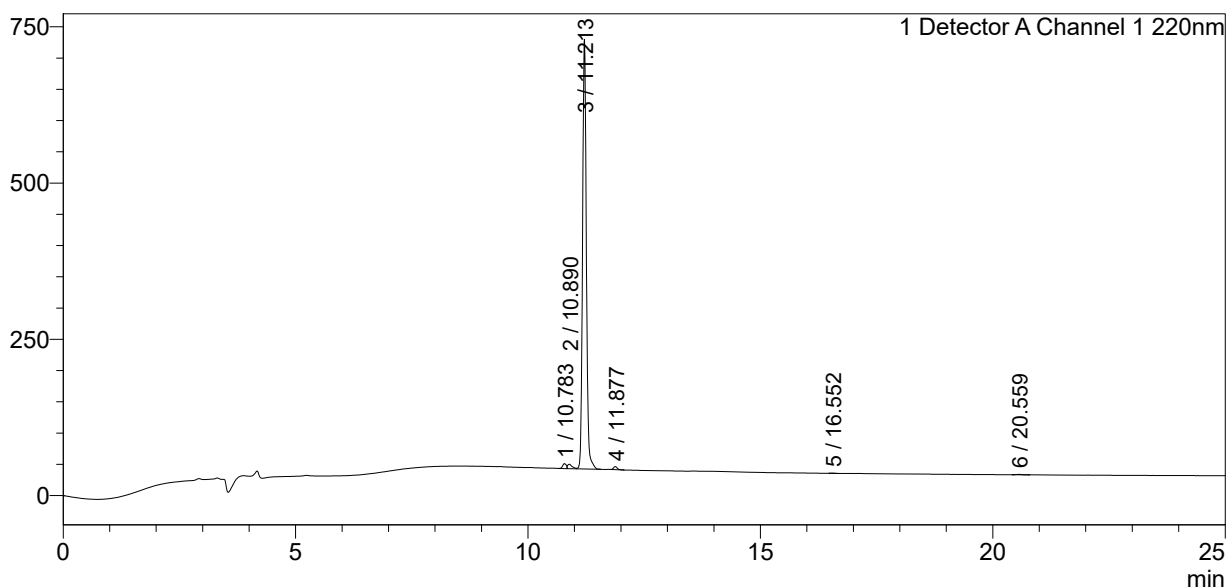

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.783	43750	7900	1.093
2	10.890	46001	7038	1.149
3	11.213	3878339	687213	96.891
4	11.877	26840	4920	0.671
5	16.552	1906	330	0.048
6	20.559	5940	736	0.148
Total		4002776	708137	100.000