

Sample Name :W Peptide, WKYMVm  
 Cat No.: RP20299  
 Lot No.: E0871219K  
 Time Processed :22:43:01  
 Month-Day-Year Processed :12/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

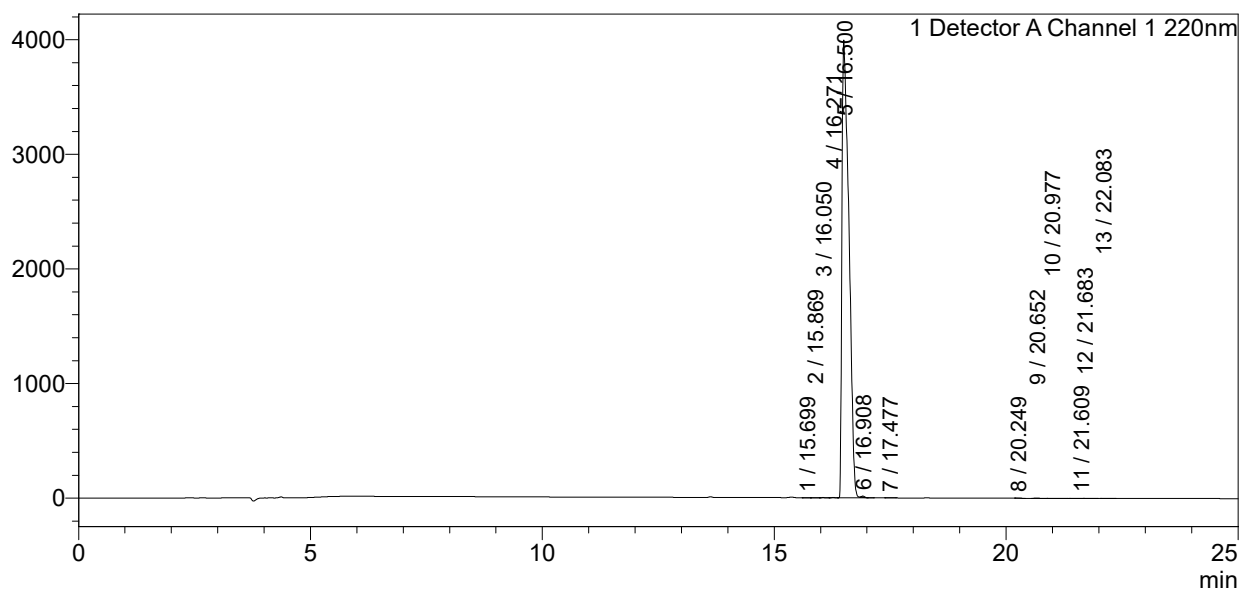

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.699	3463	616	0.008
2	15.869	6204	758	0.015
3	16.050	7890	1414	0.019
4	16.271	10759	1719	0.026
5	16.500	41530184	3995795	99.741
6	16.908	52328	12015	0.126
7	17.477	10362	1408	0.025
8	20.249	1694	335	0.004
9	20.652	6742	915	0.016
10	20.977	3651	393	0.009
11	21.609	2085	179	0.005
12	21.683	1439	174	0.003
13	22.083	1341	113	0.003
Total		41638143	4015834	100.000