

Sample Name :Amylin, human, amide  
 Cat No. :RP11278  
 Lot No. :E0677421A  
 Time Processed : 9:00:09 PM  
 Month-Day-Year Processed : 01/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	10
25.00	Pumps	Pump A B.Conc	70
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	10
40.00	Pumps	Pump A B.Conc	10
95.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

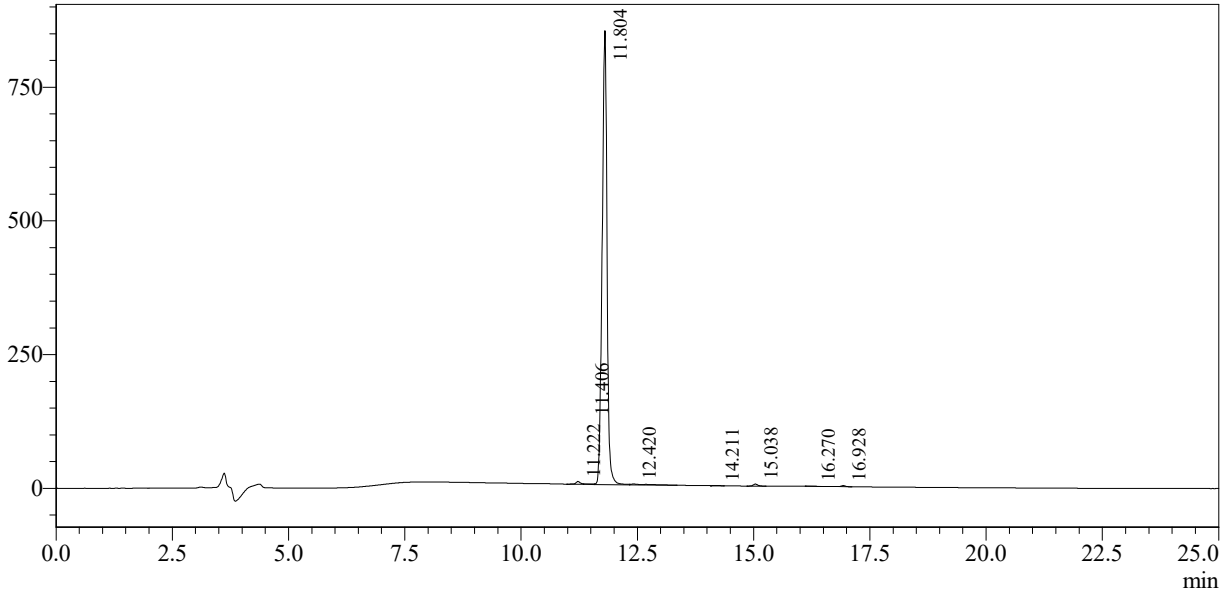

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.222	35789	5165	0.564
2	11.406	13186	1052	0.208
3	11.804	6221385	848508	97.988
4	12.420	35363	1715	0.557
5	14.211	2788	394	0.044
6	15.038	24765	3770	0.390
7	16.270	3732	478	0.059
8	16.928	12091	1952	0.190
Total		6349099	863034	100.000