

Sample Name :Hsp70-derived octapeptide  
 Cat. No. : RP20220  
 Lot. No. : PE8551905  
 Time Processed :4:46:01  
 Month-Day-Year Processed : 05/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

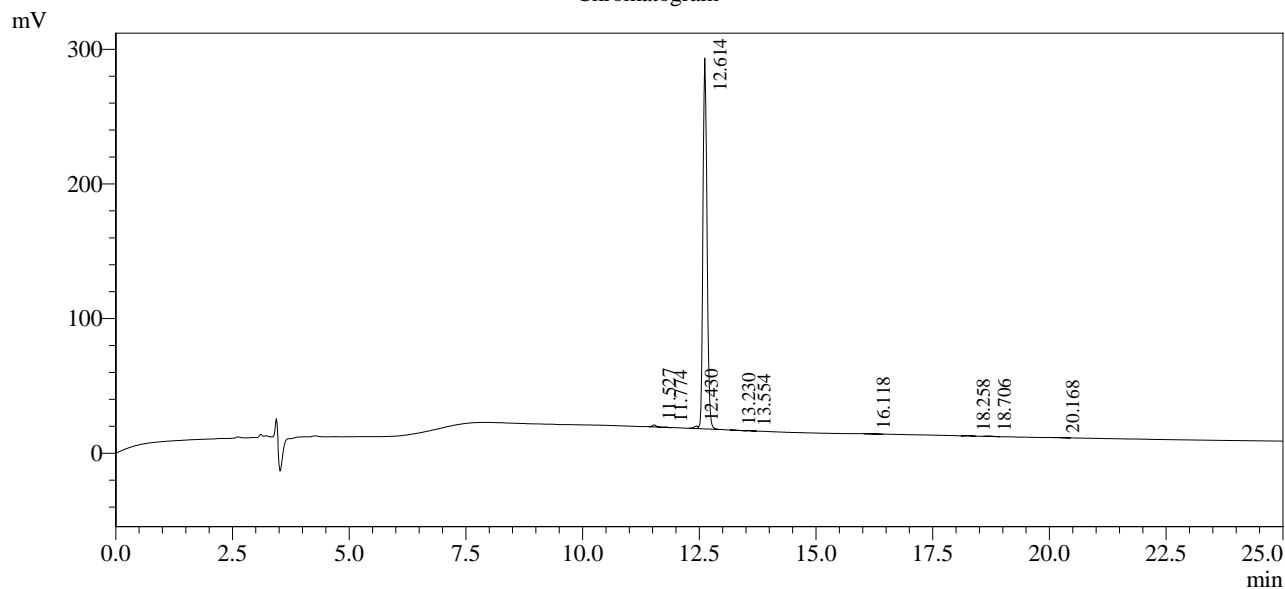

1 Det. A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.527	8853	1538	0.513
2	11.774	1914	366	0.111
3	12.430	10324	1769	0.599
4	12.614	1689672	275475	97.980
5	13.230	2030	254	0.118
6	13.554	1334	241	0.077
7	16.118	2713	278	0.157
8	18.258	2471	350	0.143
9	18.706	2956	437	0.171
10	20.168	2241	251	0.130
Total		1724508	280960	100.000