

Sample Name : TAT peptide  
 Cat. No. : RP20256  
 Lot. No. : E5858219L  
 Time Processed : 8:35:42  
 Month-Day-Year Processed : 12/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

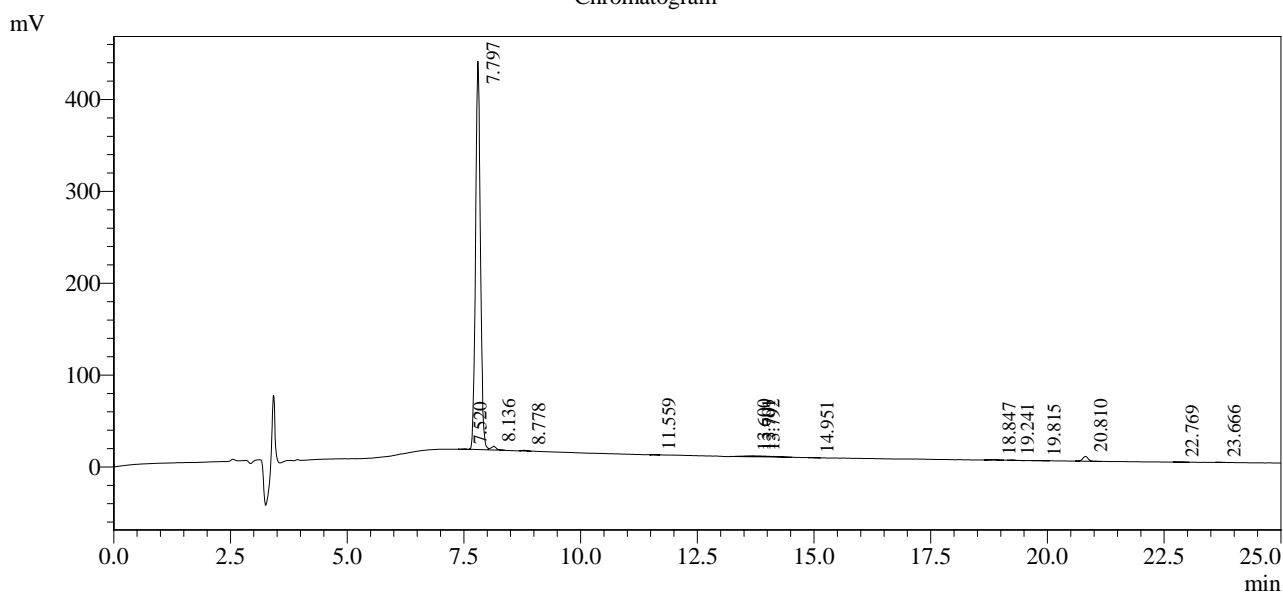

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.520	2893	519	0.090
2	7.797	3058973	422734	95.468
3	8.136	31469	4042	0.982
4	8.778	4358	746	0.136
5	11.559	1123	185	0.035
6	13.600	12224	909	0.381
7	13.701	7229	1010	0.226
8	13.792	24134	963	0.753
9	14.951	1162	144	0.036
10	18.847	8651	743	0.270
11	19.241	3958	503	0.124
12	19.815	1678	171	0.052
13	20.810	42668	5310	1.332
14	22.769	1092	120	0.034
15	23.666	2571	294	0.080
Total		3204185	438392	100.000