

Sample Name : Cortistatin 14, human, rat
 Cat.No.:RP10972 Lot.No.:PE5331711

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

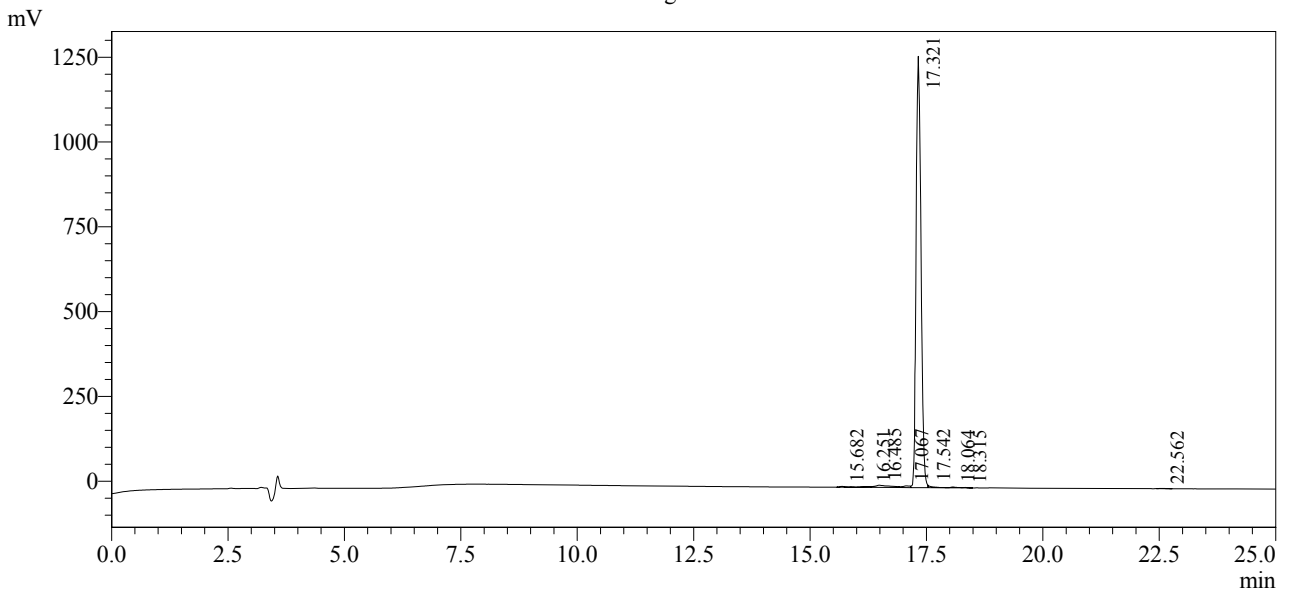

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.682	15917	2543	0.165
2	16.251	38934	2381	0.403
3	16.485	150024	6499	1.553
4	17.067	56275	5063	0.583
5	17.321	9312867	1271426	96.431
6	17.542	43605	6255	0.452
7	18.064	22097	2498	0.229
8	18.315	11221	1313	0.116
9	22.562	6624	740	0.069
Total		9657563	1298718	100.000