


# Mass Spectrum

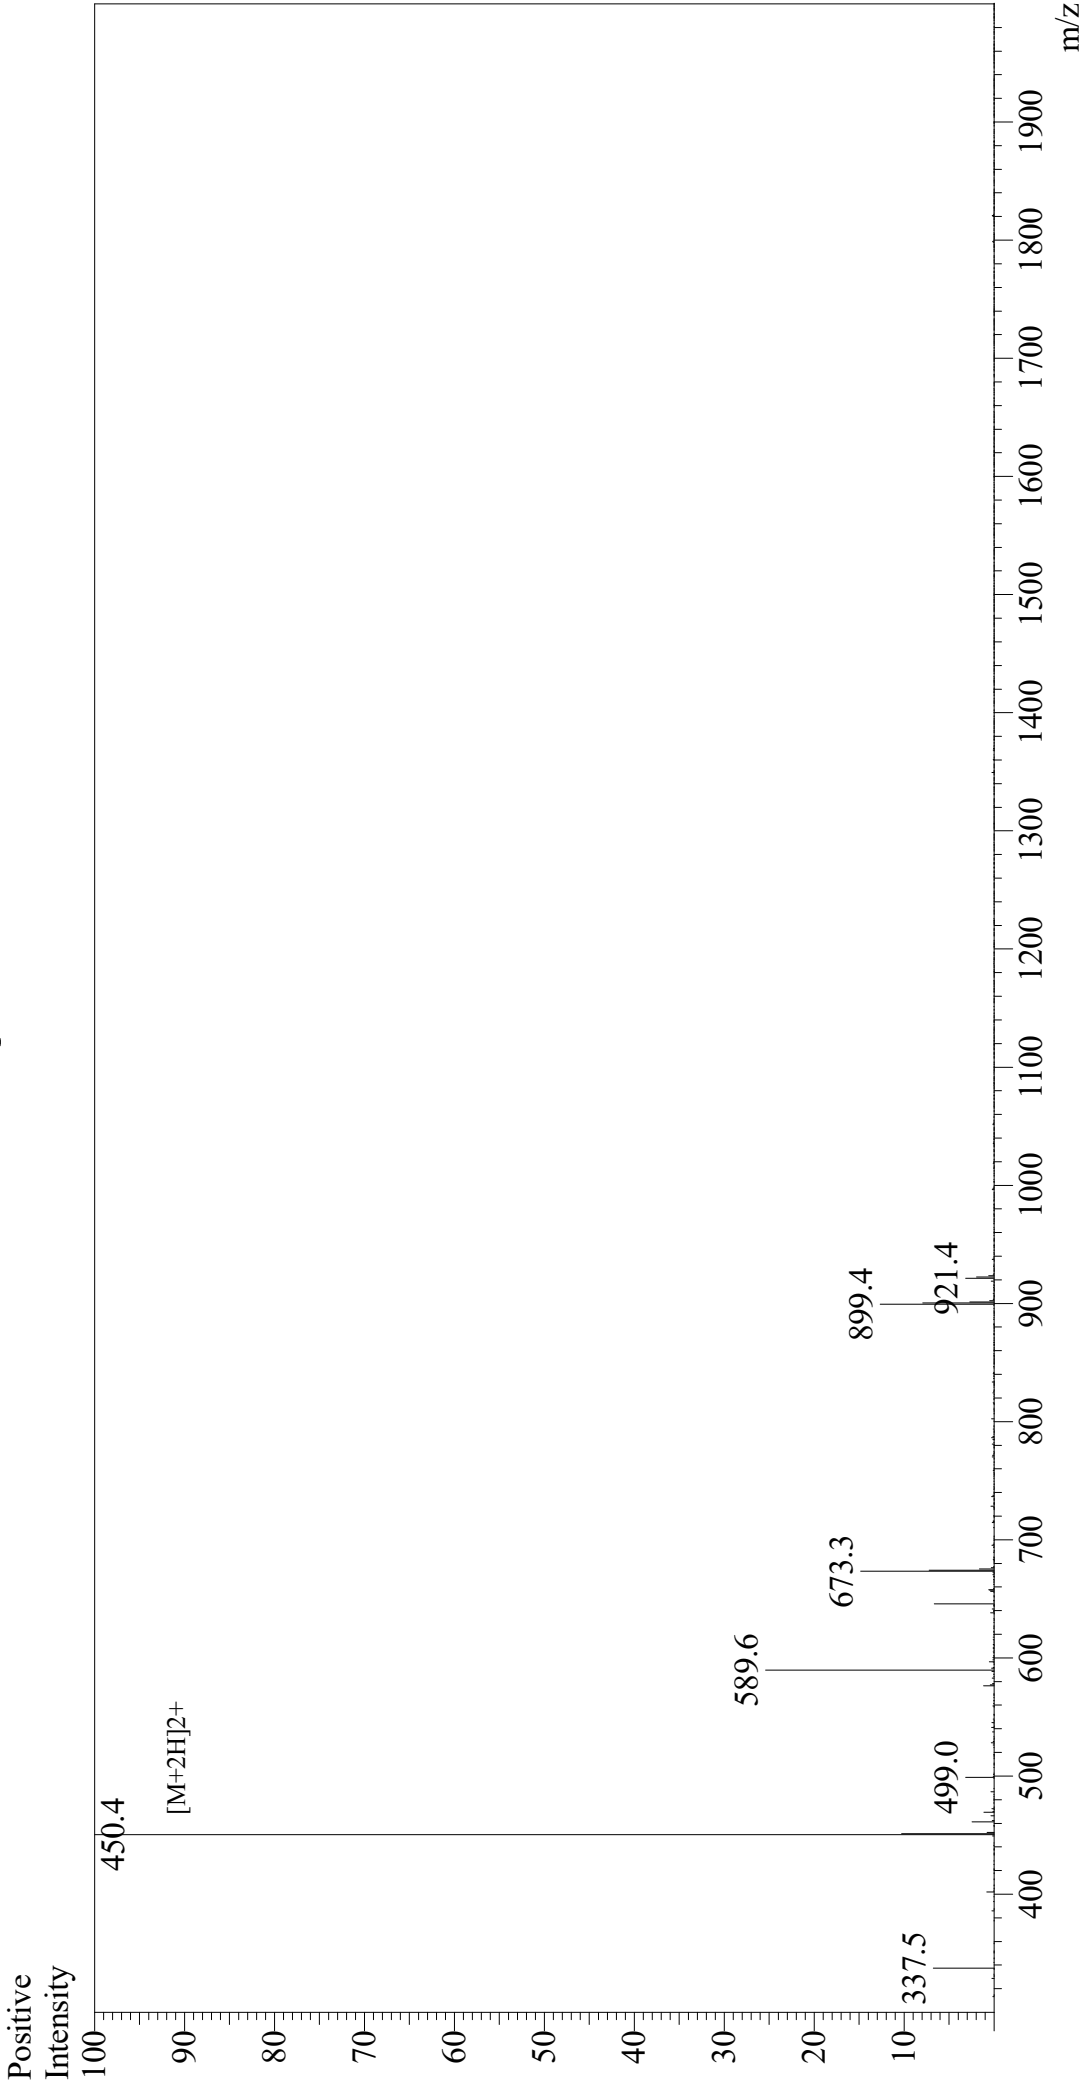

Sample Information  
Month-Day Processed : 11/03/20  
Time Processed : 09:06:01 AM  
Injection Volume : 0.3  
Sample Name : Cardiotoxin Analog (CTX) IV (6-12)  
Cat.No : RP17303  
Lot.No : E3653920J  
Theoretical MW : 899.14  
Observed MW : 898.8

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50% H2O/50% MeOH