

Sample Name : InsB 9-23  
 Cat. No. :RP20391  
 Lot. No. :PE3121701

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

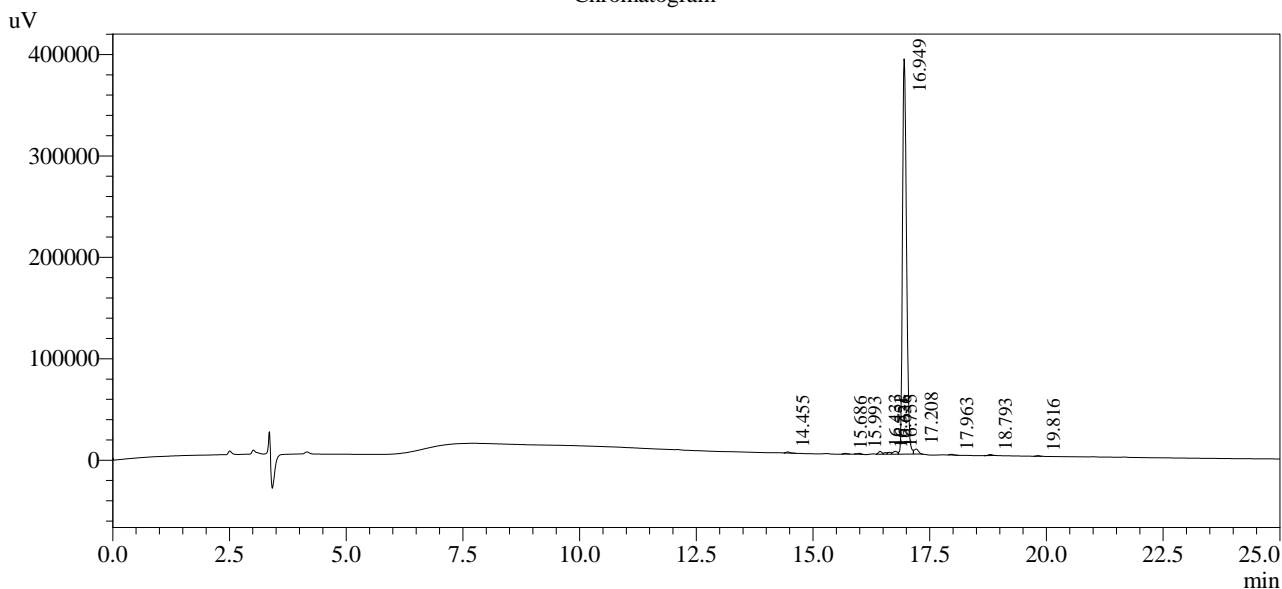

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.455	6178	1136	0.252
2	15.686	3616	763	0.148
3	15.993	6485	1024	0.265
4	16.433	14004	2802	0.572
5	16.551	7519	1533	0.307
6	16.636	8772	1816	0.358
7	16.755	18338	2783	0.749
8	16.949	2339636	389753	95.555
9	17.208	31394	4927	1.282
10	17.963	3475	711	0.142
11	18.793	6418	1019	0.262
12	19.816	2627	571	0.107
Total		2448462	408839	100.000