

Sample Name : MOG(35-55)
 Cat. No. : RP10245
 Lot. No. : E1980820E
 Time Processed : 11:48:54
 Month-Day-Year Processed : 06/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

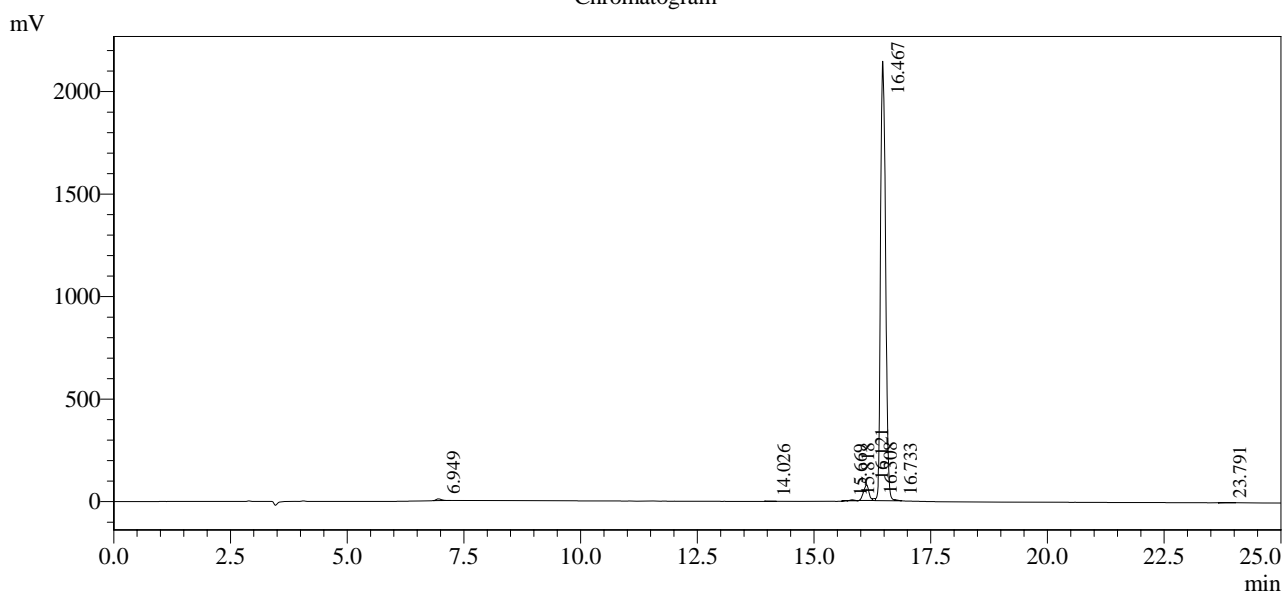

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.949	64106	8225	0.379
2	14.026	2980	543	0.018
3	15.669	4321	909	0.026
4	15.818	29325	4184	0.173
5	16.121	607954	76707	3.592
6	16.308	36557	9515	0.216
7	16.467	16153473	2142047	95.432
8	16.733	16710	4519	0.099
9	23.791	11237	1188	0.066
Total		16926662	2247837	100.000