

Sample Name :  $\beta$ -Amyloid (1-40)  
 Cat No.: RP20528  
 Lot No.:E7956320A  
 Time Processed :15:12:03  
 Month-Day-Year Processed :01/17/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	15
25.00	Pumps	Solvent B Conc.	75
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	15
40.00	Pumps	Solvent B Conc.	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

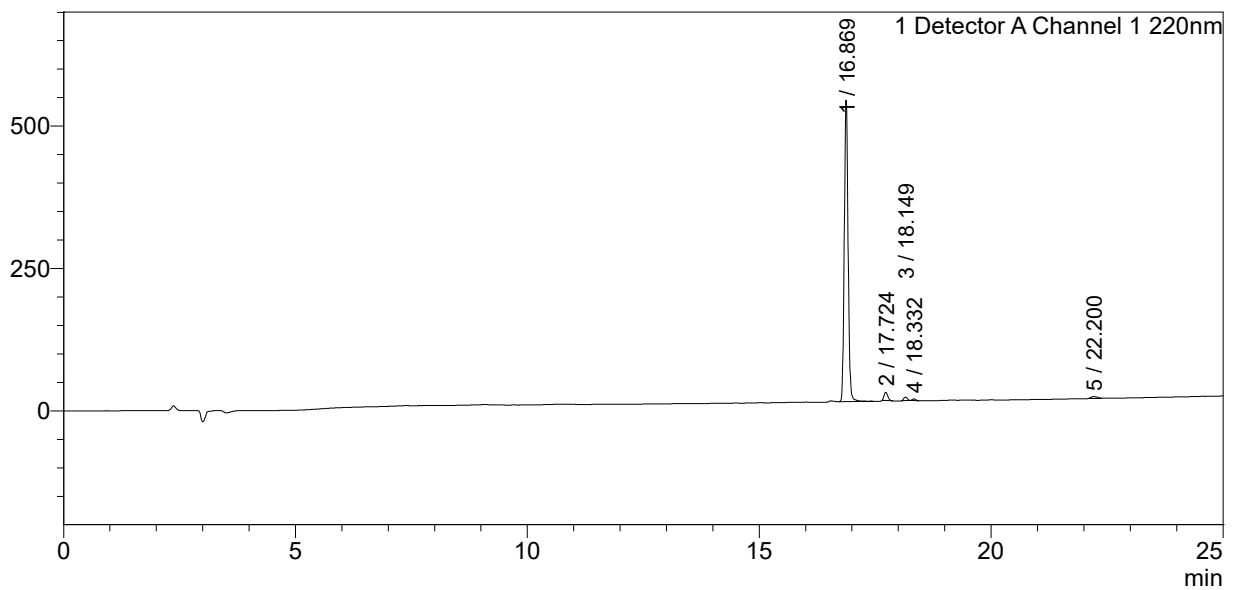

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.869	3012606	529353	95.085
2	17.724	79976	14575	2.524
3	18.149	31496	5990	0.994
4	18.332	12564	2797	0.397
5	22.200	31697	3118	1.000
Total		3168339	555833	100.000