

Sample Name: GnRH-I
 Cat No. : RP20303
 Lot No. : E6996420A
 Time Processed: 9:27:29 PM
 Month-Day-Year Processed :01/21/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

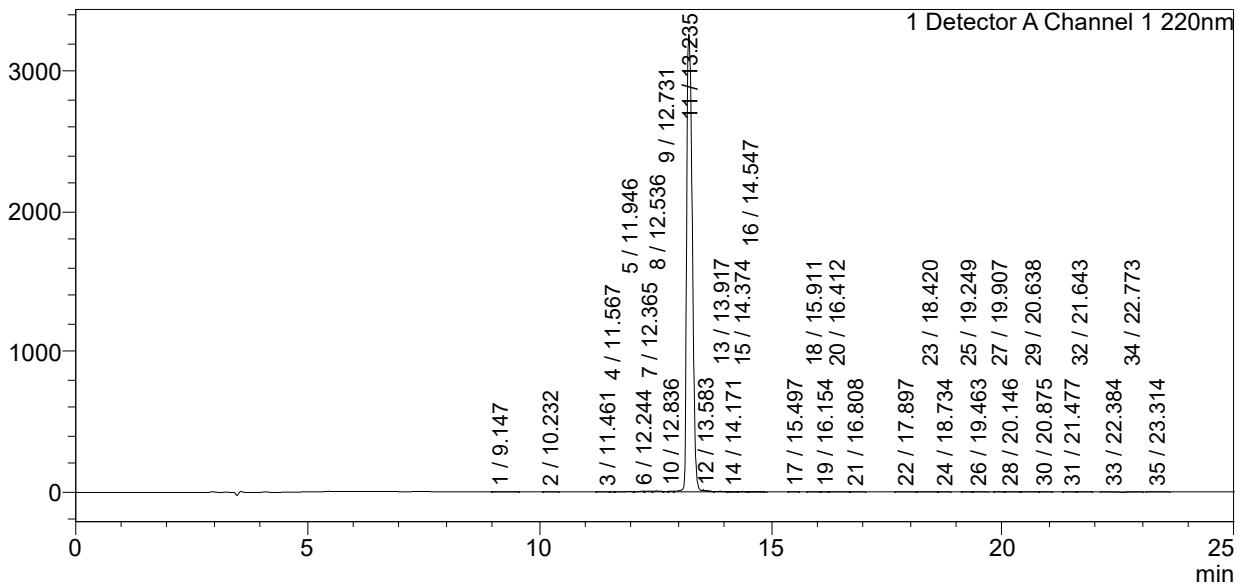

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.147	5662	320	0.020
2	10.232	1731	158	0.006
3	11.461	4622	437	0.017
4	11.567	1736	394	0.006
5	11.946	28629	2377	0.102
6	12.244	41298	5276	0.148
7	12.365	51067	5799	0.183
8	12.536	66932	6373	0.239
9	12.731	13493	3461	0.048
10	12.836	33964	4892	0.121
11	13.235	27606041	3261691	98.707
12	13.583	12814	2182	0.046
13	13.917	15129	2253	0.054
14	14.171	2709	516	0.010

Peak#	Ret. Time	Area	Height	Area%
15	14.374	18163	3163	0.065
16	14.547	7025	712	0.025
17	15.497	2981	503	0.011
18	15.911	1496	162	0.005
19	16.154	2982	517	0.011
20	16.412	3864	269	0.014
21	16.808	1261	107	0.005
22	17.897	2894	173	0.010
23	18.420	4402	320	0.016
24	18.734	2045	183	0.007
25	19.249	1235	130	0.004
26	19.463	2963	190	0.011
27	19.907	1480	154	0.005
28	20.146	3145	340	0.011
29	20.638	2111	127	0.008
30	20.875	1094	118	0.004
31	21.477	6178	625	0.022
32	21.643	2631	289	0.009
33	22.384	2767	204	0.010
34	22.773	6503	648	0.023
35	23.314	4683	365	0.017
Total		27967728	3305427	100.000