

Sample Name : C-Myc Peptide
 Cat No : RP11731
 Lot No : E5280221D
 Time Processed : 2:26:46 AM
 Month-Day-Year Processed : 04/19/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : GK11010011

<Chromatogram>

mV

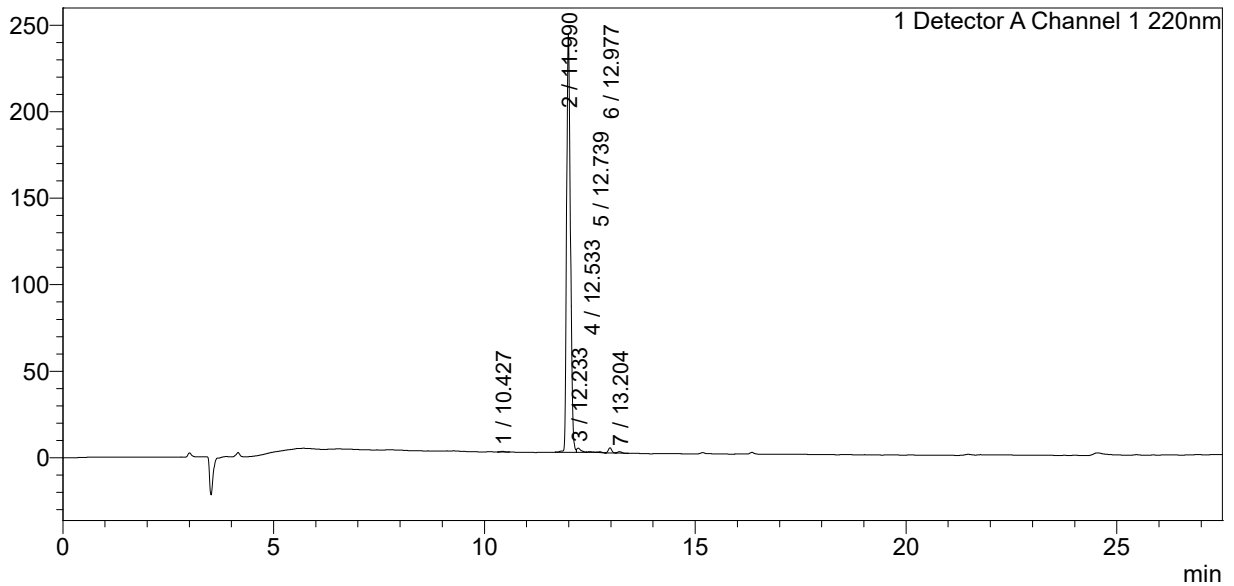

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.427	2403	368	0.152
2	11.990	1536544	238212	97.272
3	12.233	15154	2312	0.959
4	12.533	2215	238	0.140
5	12.739	2218	393	0.140
6	12.977	16204	2900	1.026
7	13.204	4897	779	0.310
Total		1579636	245202	100.000