

Sample Name : Ghrelin, rat  
 Cat. No. : RP10781  
 Lot. No. : E6399020C  
 Time Processed : 12:52:26  
 Month-Day-Year Processed : 03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

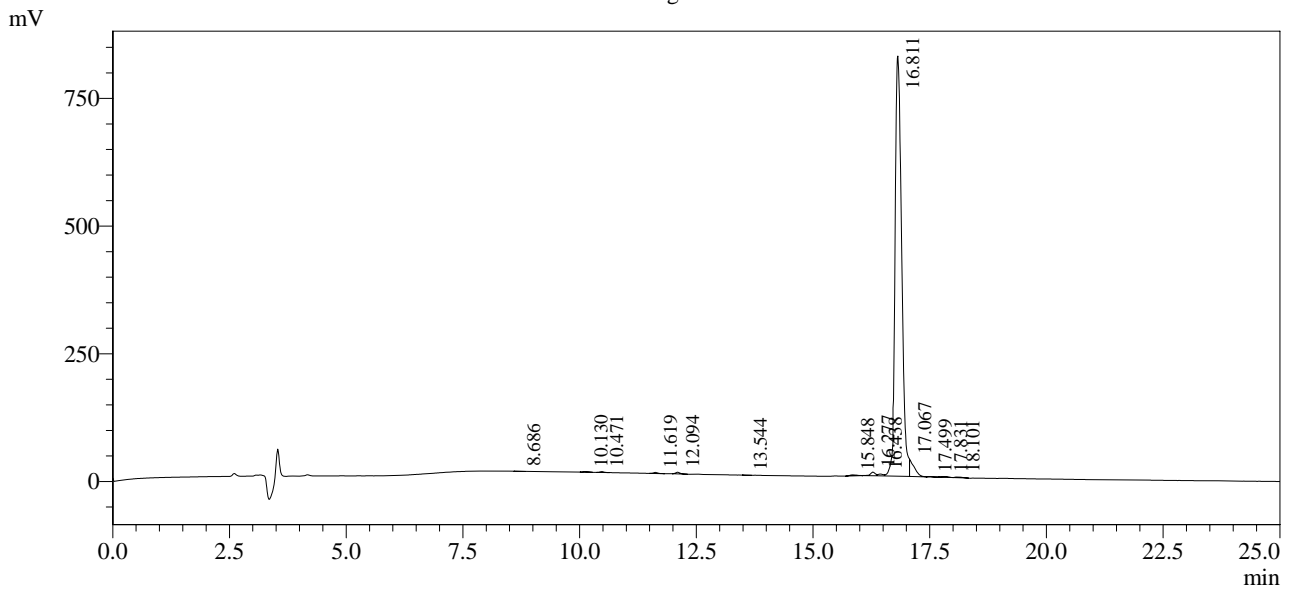

1 Det.A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.686	3781	631	0.044
2	10.130	8323	1223	0.098
3	10.471	9617	1635	0.113
4	11.619	12308	2010	0.145
5	12.094	20349	3188	0.239
6	13.544	1053	174	0.012
7	15.848	17895	1742	0.210
8	16.277	51360	7086	0.604
9	16.438	28606	3593	0.336
10	16.811	8093895	822997	95.159
11	17.067	227508	34218	2.675
12	17.499	5266	961	0.062
13	17.831	12365	1442	0.145
14	18.101	13366	1486	0.157
Total		8505692	882386	100.000