

Sample Name :OVA Peptide (323-339)
 Cat No.: RP10610
 Lot No.: E00625201
 Time Processed :23:23:23
 Month-Day-Year Processed :09/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

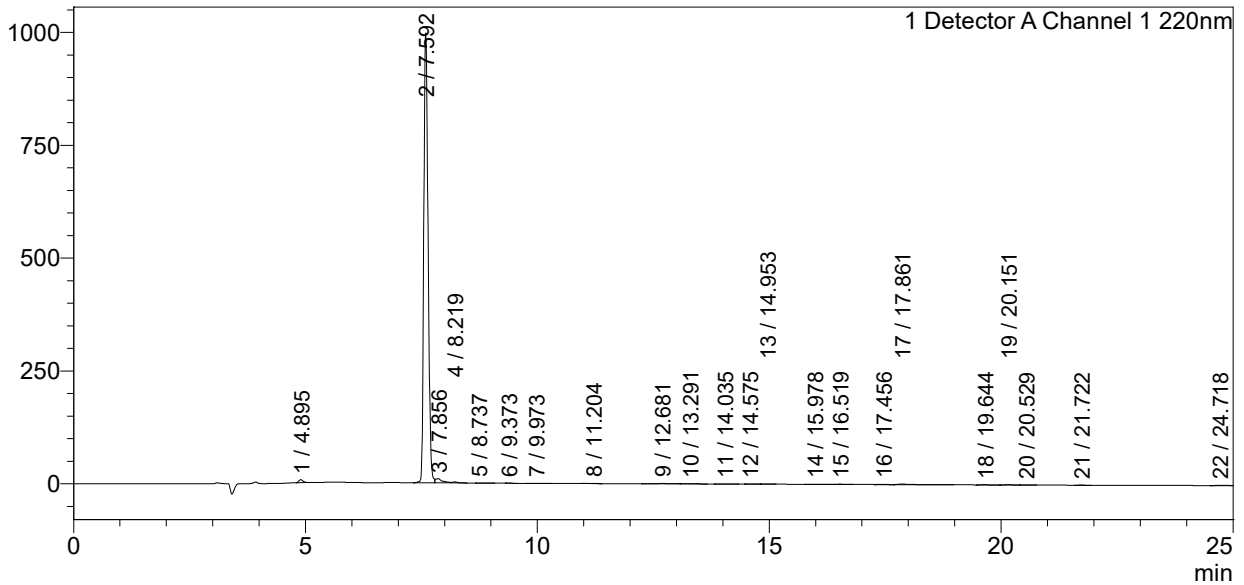

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	4.895	40232	6392	0.601
2	7.592	6446360	996662	96.221
3	7.856	96460	9128	1.440
4	8.219	19053	2186	0.284
5	8.737	2198	157	0.033
6	9.373	1012	133	0.015
7	9.973	1933	118	0.029
8	11.204	3413	394	0.051
9	12.681	15064	608	0.225
10	13.291	7011	368	0.105
11	14.035	6527	343	0.097
12	14.575	1041	97	0.016
13	14.953	1209	114	0.018
14	15.978	7302	301	0.109
15	16.519	5155	538	0.077

Peak#	Ret. Time	Area	Height	Area%
16	17.456	2678	216	0.040
17	17.861	24836	1276	0.371
18	19.644	2267	150	0.034
19	20.151	3053	250	0.046
20	20.529	2277	233	0.034
21	21.722	1959	228	0.029
22	24.718	8530	780	0.127
Total		6699570	1020672	100.000