

Sample Name :Gly-Arg-Gly-Asp-Ser
 Cat No. :RP10848
 Lot No. :E9402921D
 Time Processed :4:32:40 PM
 Month-Day-Year Processed :04/22/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------|-------|
| 0.01 | Pumps | B.Conc | 0 |
| 5.00 | Pumps | B.Conc | 0 |
| 20.00 | Pumps | B.Conc | 30 |
| 25.00 | Pumps | B.Conc | 65 |
| 25.01 | Pumps | B.Conc | 95 |
| 27.00 | Pumps | B.Conc | 95 |
| 27.01 | Pumps | B.Conc | 0 |
| 35.00 | Pumps | B.Conc | 0 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

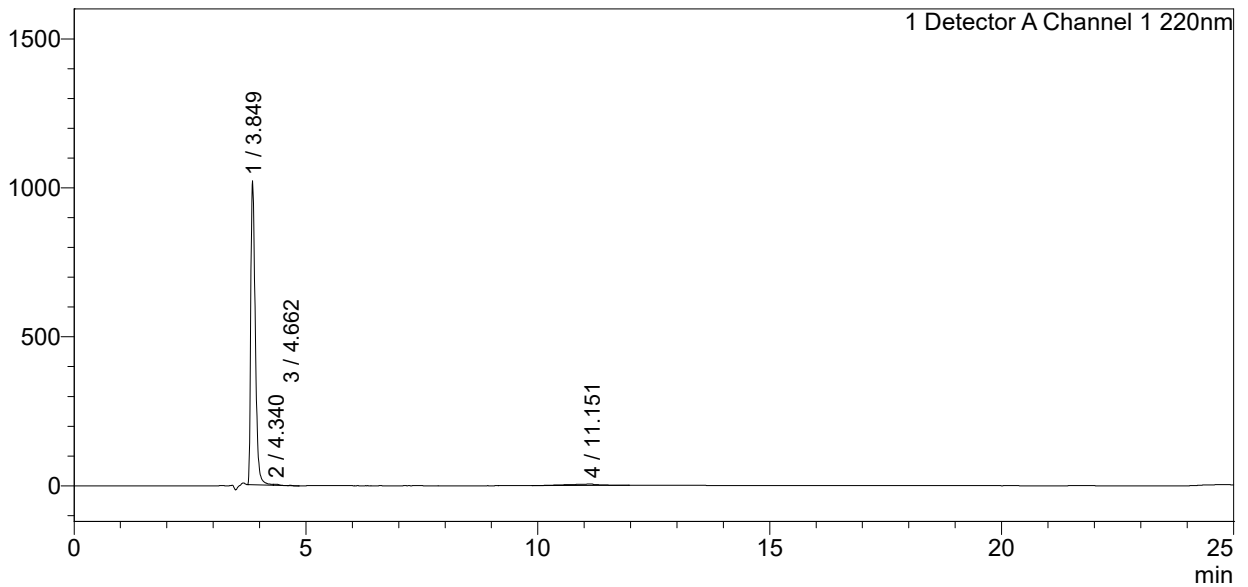

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|---------|---------|
| 1 | 3.849 | 6883021 | 1019251 | 96.597 |
| 2 | 4.340 | 25631 | 3535 | 0.360 |
| 3 | 4.662 | 3115 | 1254 | 0.044 |
| 4 | 11.151 | 213707 | 4493 | 2.999 |
| Total | | 7125474 | 1028533 | 100.000 |