

Sample Name :hgp100(25-33)
 Cat. No. : RP20344
 Lot. No. :E492319I
 Time Processed :11:15:31
 Month-Day-Year Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

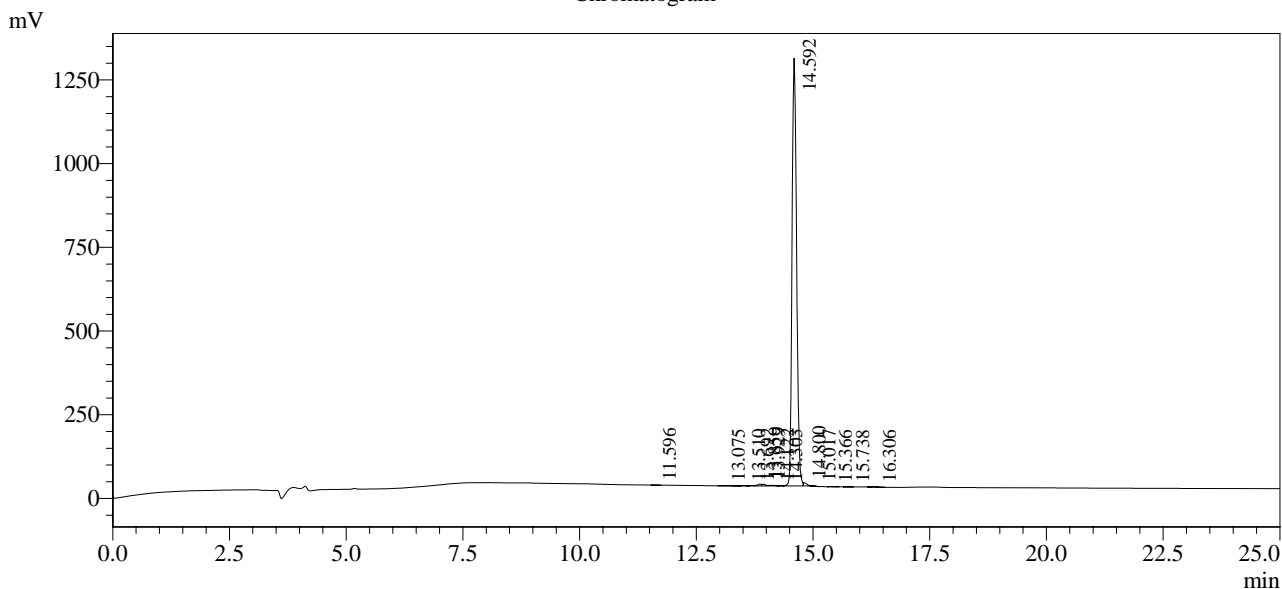

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.596	1971	309	0.022
2	13.075	6362	391	0.072
3	13.510	7505	1185	0.084
4	13.692	8377	1430	0.094
5	13.859	32976	5293	0.371
6	13.929	30078	5253	0.338
7	14.122	17924	2102	0.202
8	14.303	3565	722	0.040
9	14.592	8712859	1277548	98.012
10	14.800	47688	9744	0.536
11	15.017	6850	1443	0.077
12	15.366	2588	470	0.029
13	15.738	2293	418	0.026
14	16.306	8507	1453	0.096
Total		8889544	1307763	100.000