

Sample Name : Osteogenic Growth Peptide,OGP
 Cat. No. : RP20311
 Lot. No. : PE8741903
 Time Processed : 6:17:25
 Month-Day-Year Processed : 03/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

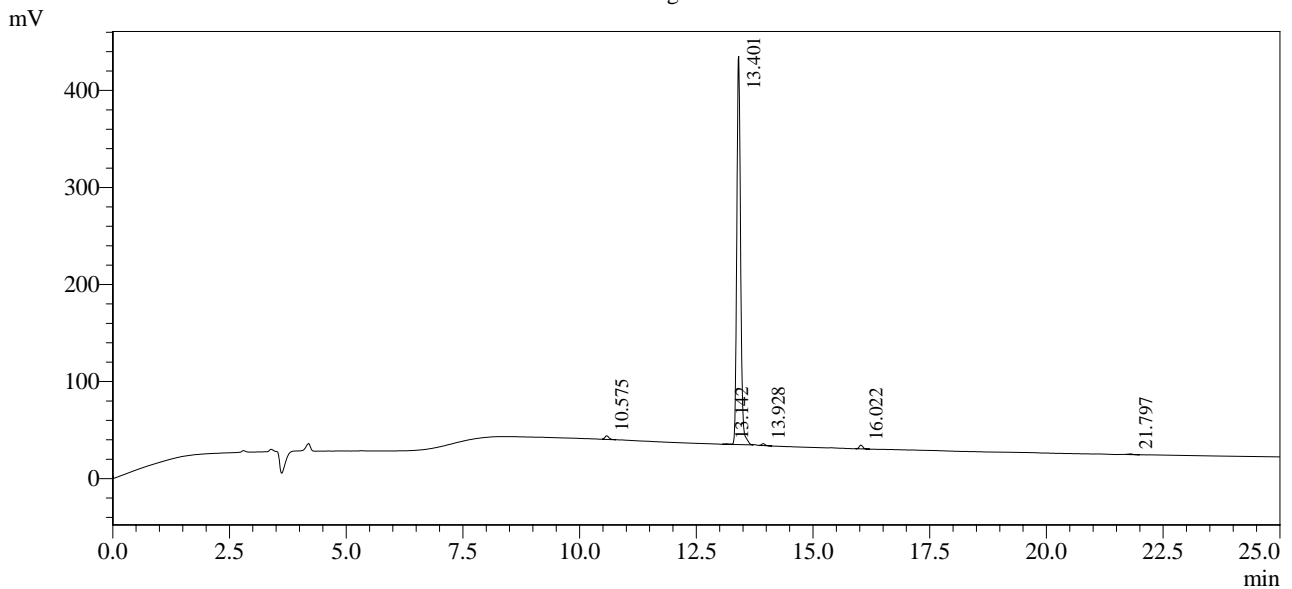

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.575	21518	3690	0.925
2	13.142	3243	409	0.139
3	13.401	2265338	400156	97.362
4	13.928	10743	2036	0.462
5	16.022	21490	3956	0.924
6	21.797	4397	731	0.189
Total		2326728	410978	100.000