


Mass Spectrum

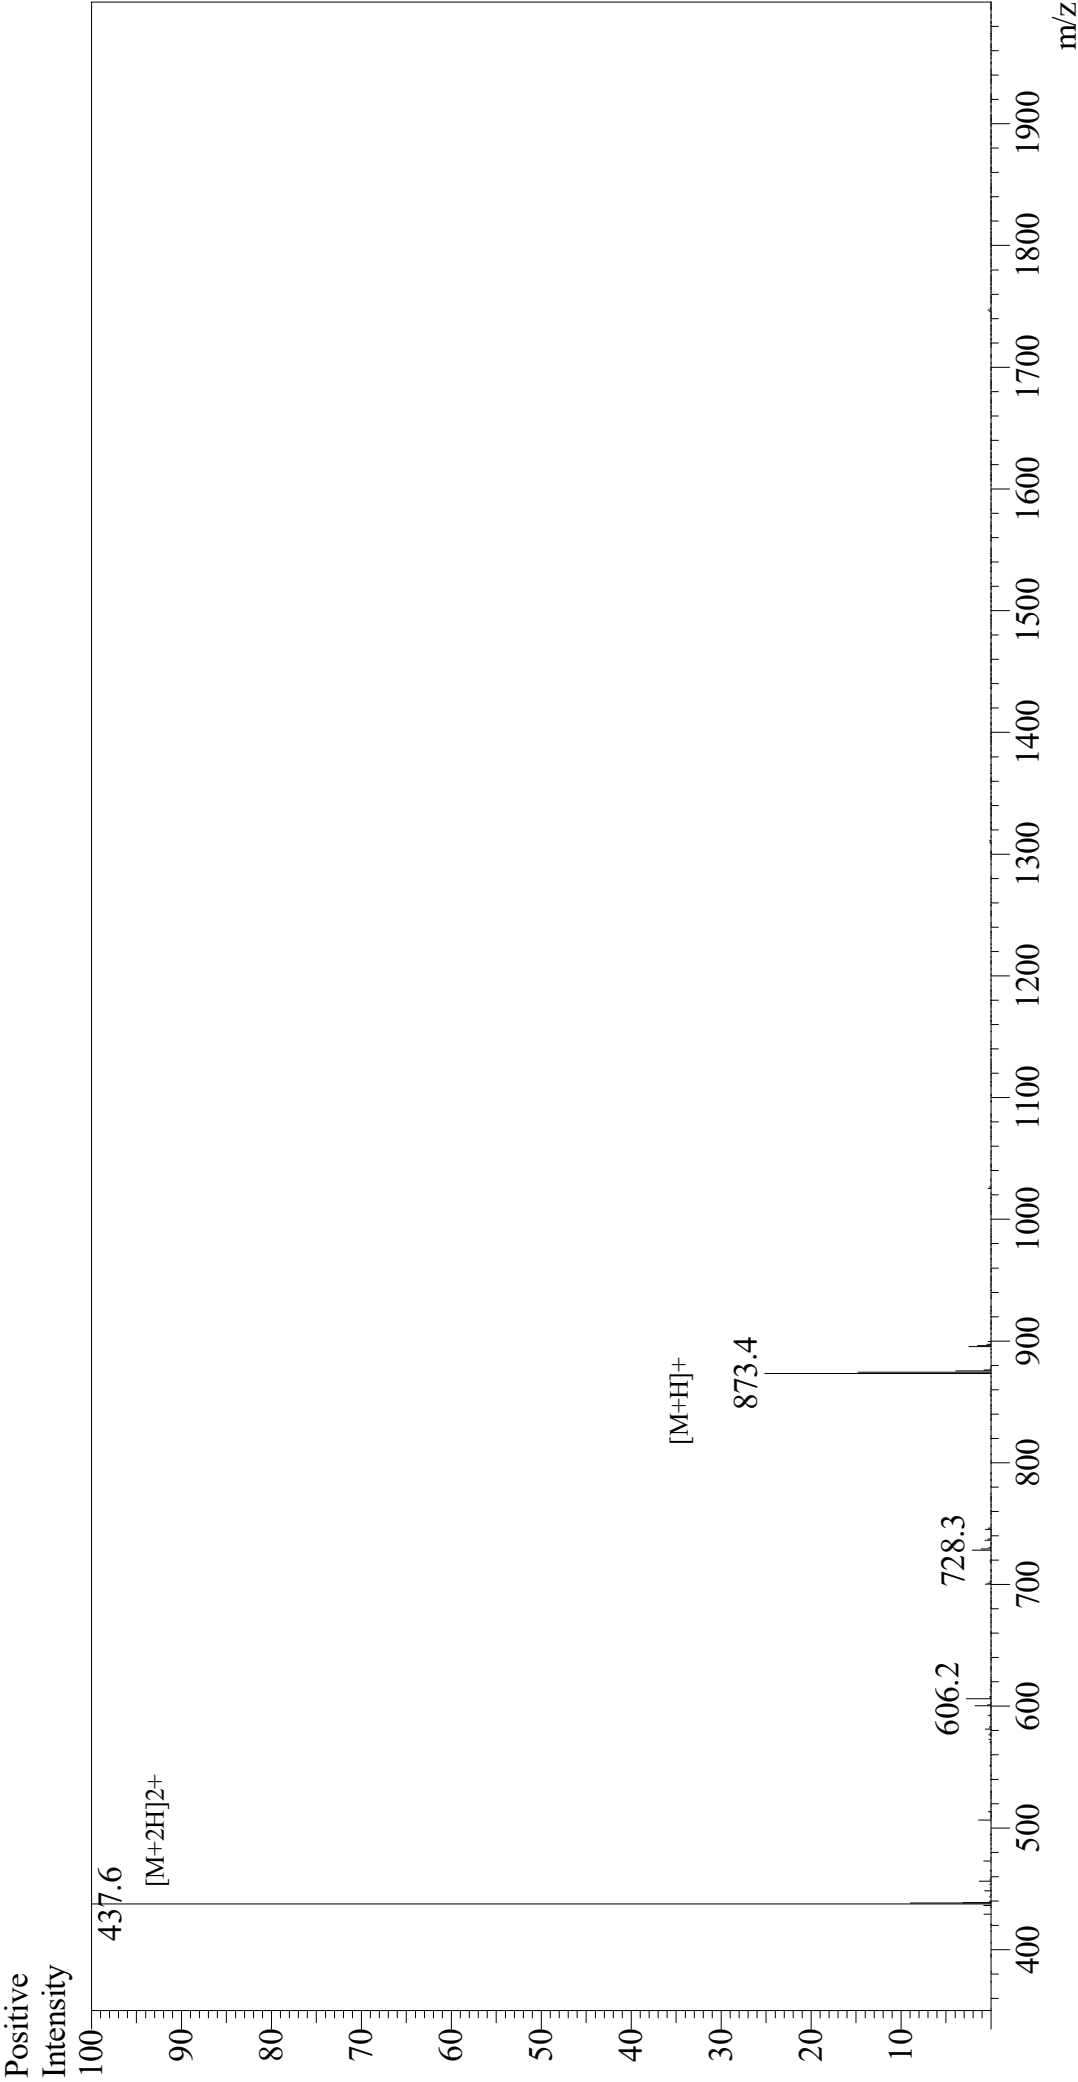

Sample Information

Month-Day Processed :	08/12/21	Equipment	: ZJ21010035
Time Processed :	22:44:10	Interface Bias	: +4.5 kV
Injection Volume :	0.4	Drying Gas Flow	: 5 L/min
Sample Name :	Growth Hormone Releasing Factor (GHRF)-6	T.Flow	: 0.2 ml/min
Cat. No. :	RP10741	B.conc	: 50% H ₂ O/50% MeOH
Lot. No. :	E5845821H		
Theoretical MW :	873.00		
Observed MW :	873.2		