

Sample Name :Kisspeptin-10
 Cat No. :RP20494
 Lot No. :E0909019G
 Time Processed :8:25:48
 Month-Day-Year Processed :07/02/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

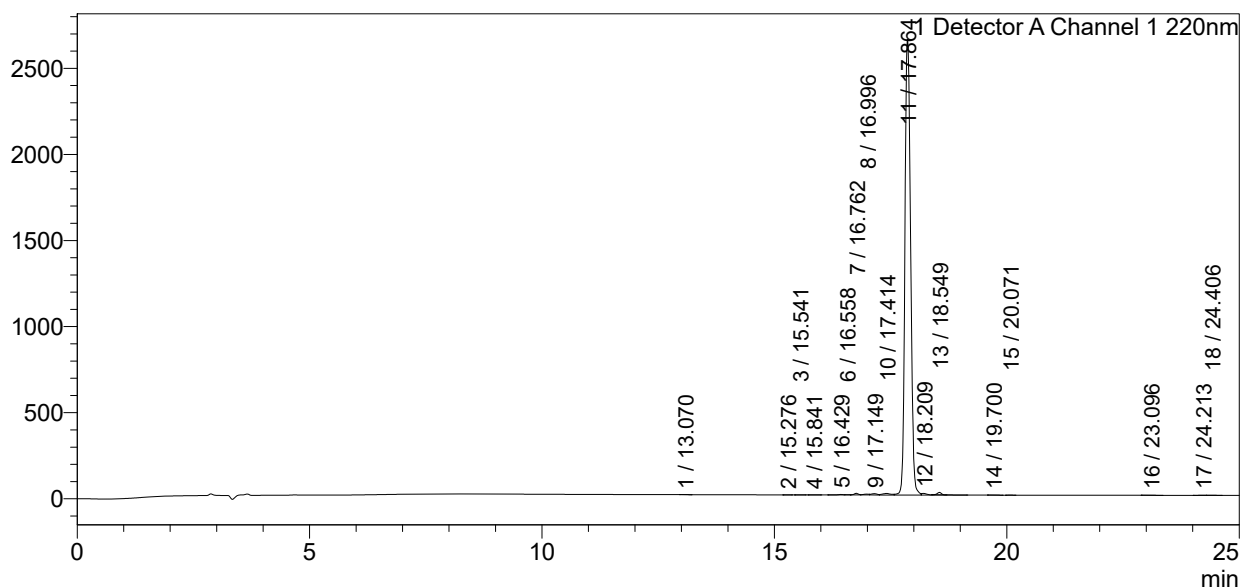

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.070	2828	462	0.012
2	15.276	1606	334	0.007
3	15.541	1151	179	0.005
4	15.841	2425	384	0.011
5	16.429	21645	2674	0.095
6	16.558	8051	1384	0.035
7	16.762	60528	9454	0.265
8	16.996	43114	4988	0.188
9	17.149	66646	7627	0.291
10	17.414	111709	8881	0.488
11	17.864	22350957	2645869	97.704
12	18.209	96050	9569	0.420
13	18.549	90372	14373	0.395
14	19.700	4493	649	0.020
15	20.071	1463	233	0.006

Peak#	Ret. Time	Area	Height	Area%
16	23.096	2052	219	0.009
17	24.213	5131	555	0.022
18	24.406	5884	564	0.026
Total		22876104	2708400	100.000