

Sample Name :  $\beta$ -Melanocyte Stimulating Hormone (MSH), human  
 Cat No.: RP10648  
 Lot No.:E5805420C  
 Time Processed :15:20:23  
 Month-Day-Year Processed :03/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
25.00	Pumps	Solvent B Conc.	60
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

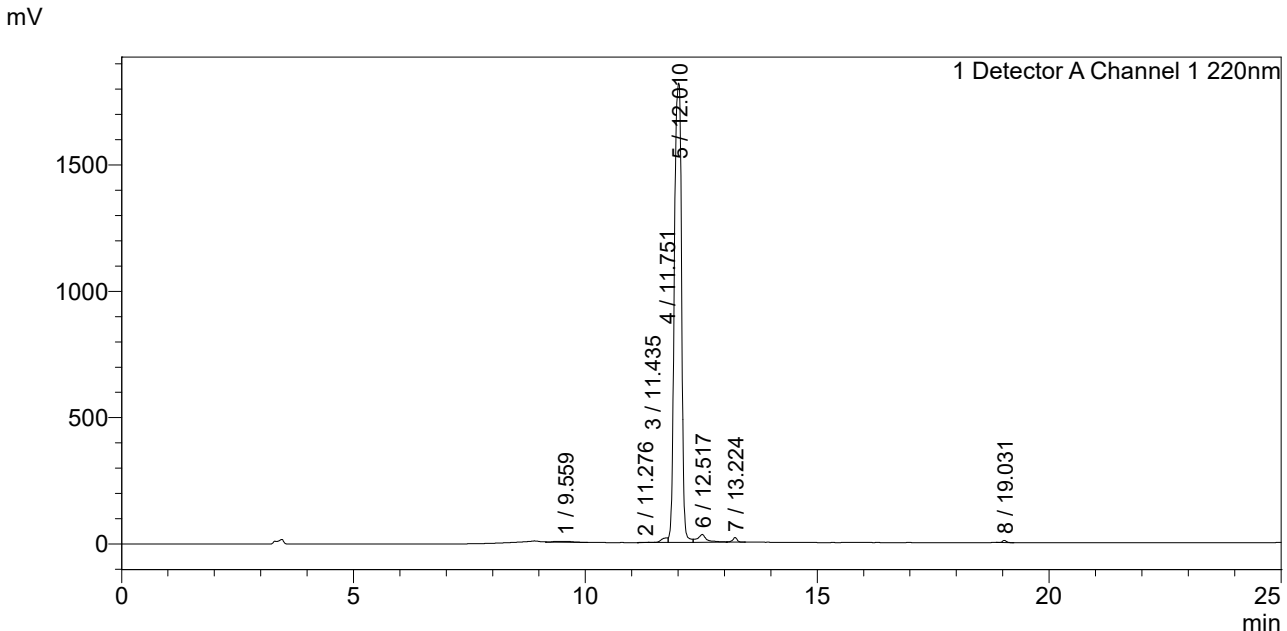

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.559	77345	3339	0.382
2	11.276	8266	848	0.041
3	11.435	5113	784	0.025
4	11.751	177763	18204	0.878
5	12.010	19378352	1818115	95.671
6	12.517	434726	31095	2.146
7	13.224	122590	18489	0.605
8	19.031	51027	8896	0.252
Total		20255182	1899771	100.000