

Sample Name :β-catenin peptide
 Cat No.:RP20466
 Lot No.:E4986119I
 Time Processed :6:34:42
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

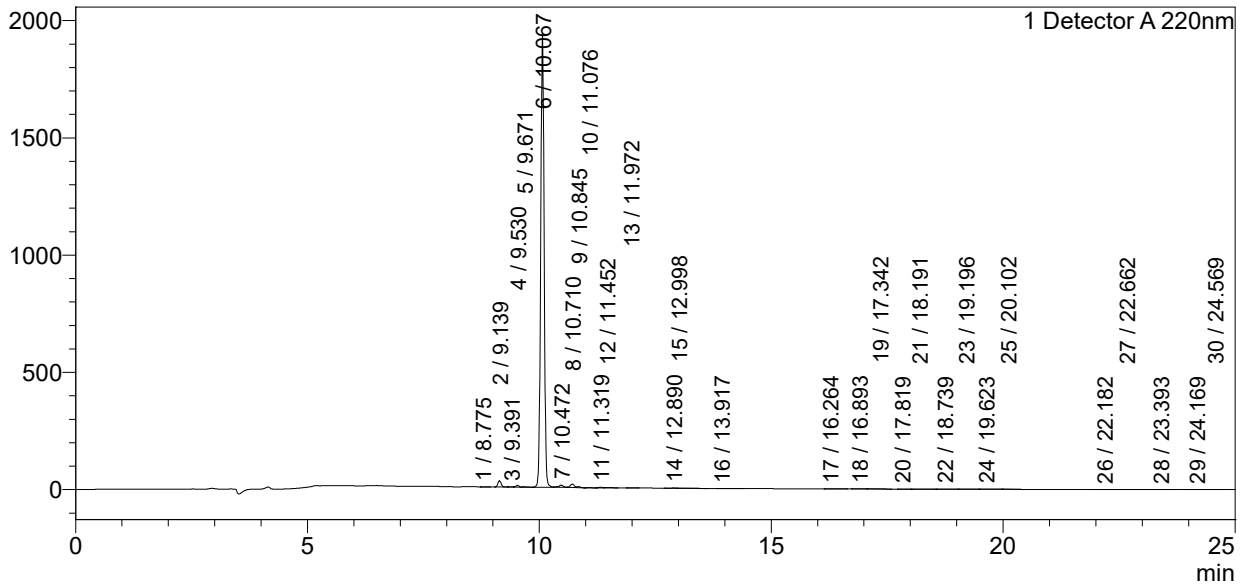

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.775	1302	145	0.013
2	9.139	131051	27109	1.259
3	9.391	3105	686	0.030
4	9.530	34214	6977	0.329
5	9.671	10754	1783	0.103
6	10.067	9968189	1937601	95.748
7	10.472	58130	9189	0.558
8	10.710	85317	14809	0.819
9	10.845	19537	4037	0.188
10	11.076	6240	1064	0.060
11	11.319	15127	2744	0.145
12	11.452	10618	987	0.102
13	11.972	3063	388	0.029
14	12.890	10128	1471	0.097
15	12.998	15503	967	0.149

Peak#	Ret. Time	Area	Height	Area%
16	13.917	3204	161	0.031
17	16.264	4039	170	0.039
18	16.893	1198	121	0.012
19	17.342	5093	332	0.049
20	17.819	1577	155	0.015
21	18.191	2643	149	0.025
22	18.739	2779	190	0.027
23	19.196	2718	199	0.026
24	19.623	1620	115	0.016
25	20.102	1045	82	0.010
26	22.182	2923	219	0.028
27	22.662	2696	157	0.026
28	23.393	2319	174	0.022
29	24.169	2989	202	0.029
30	24.569	1793	153	0.017
Total		10410911	2012536	100.000