

Sample Name : LSKL, Inhibitor of Thrombospondin (TSP-1)
 Cat. No. : RP19990
 Lot. No. : PE1861610


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

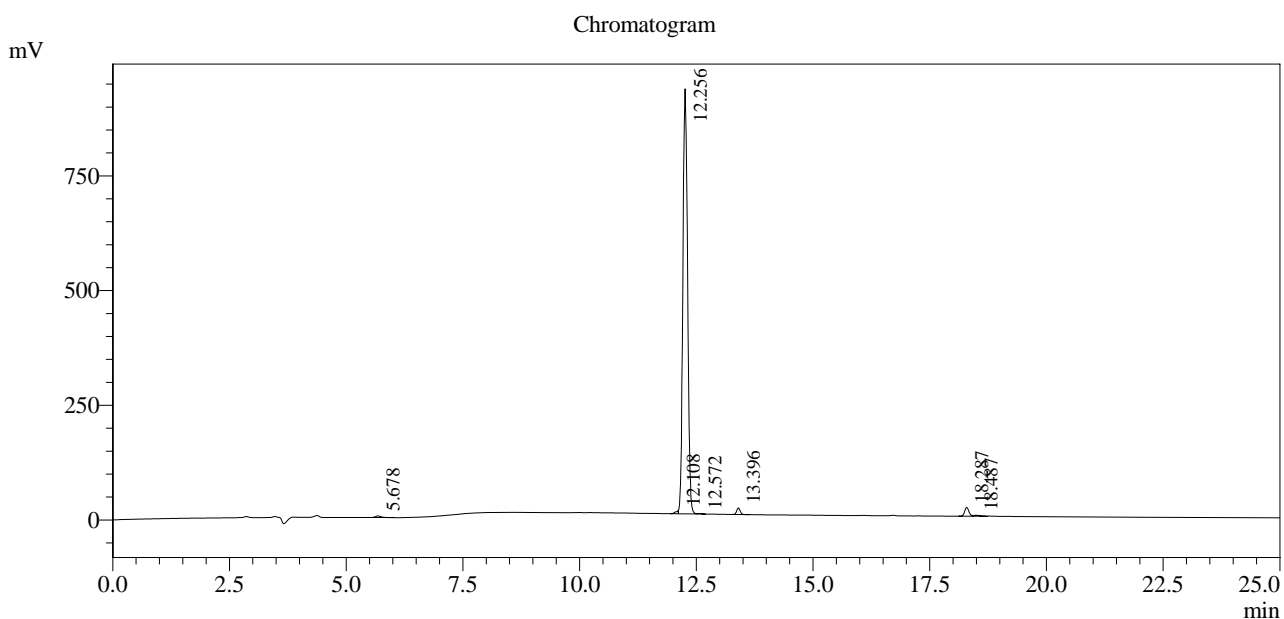

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.678	25484	3360	0.376
2	12.108	29361	6367	0.433
3	12.256	6511674	926394	95.966
4	12.572	6013	1090	0.089
5	13.396	74472	14349	1.098
6	18.287	121130	19096	1.785
7	18.487	17234	2053	0.254
Total		6785368	972709	100.000