

Sample Name :Hexa-His  
 Cat No. : RP11737  
 Lot No. :E4725819I  
 Time Processed : 2:14:06  
 Month-Day-Year Processed : 09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command      | Value |
|-------|------------|--------------|-------|
| 0.01  | Pumps      | Pump B Conc. | 0     |
| 5.00  | Pumps      | Pump B Conc. | 0     |
| 20.00 | Pumps      | Pump B Conc. | 30    |
| 25.00 | Pumps      | Pump B Conc. | 65    |
| 25.01 | Pumps      | Pump B Conc. | 95    |
| 31.00 | Pumps      | Pump B Conc. | 95    |
| 31.01 | Pumps      | Pump B Conc. | 0     |
| 40.00 | Pumps      | Pump B Conc. | 0     |
| 40.01 | Controller | Stop         |       |

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

### <Chromatogram>

mV

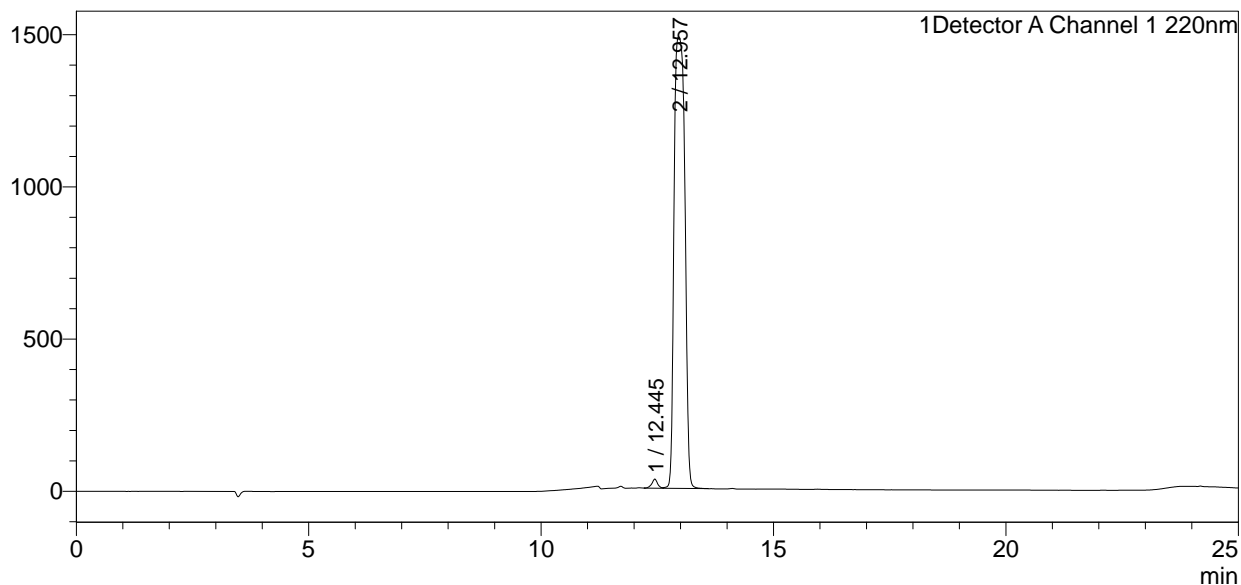

### <Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area     | Height  | Area%   |
|-------|-----------|----------|---------|---------|
| 1     | 12.445    | 260386   | 30234   | 1.082   |
| 2     | 12.957    | 23812979 | 1483601 | 98.918  |
| Total |           | 24073365 | 1513836 | 100.000 |