

Sample Name : Pep-1 (uncapped)
 Cat. No.: RP10130
 Lot. No. :E7109919J
 Time Processed :15:05:21
 Month-Day-Year Processed :10/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	0	
25.00	Pumps	Pump B Conc.	60	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

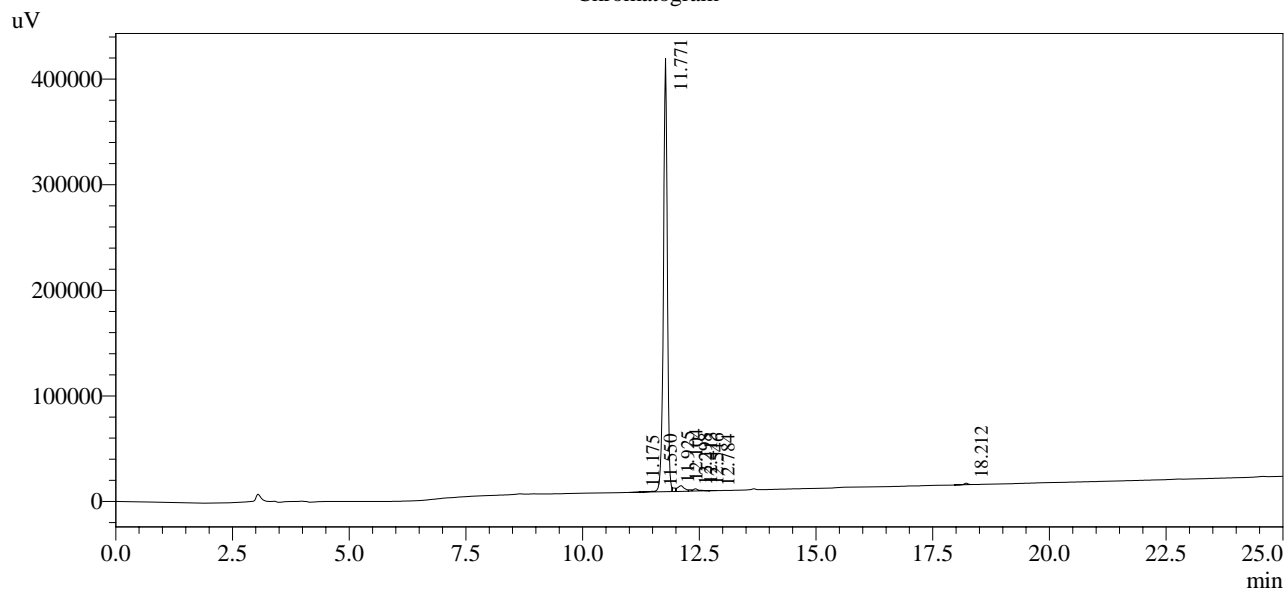

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.175	704	114	0.028
2	11.550	6214	714	0.250
3	11.771	2370378	410527	95.531
4	11.925	16516	3586	0.666
5	12.104	54028	5301	2.177
6	12.298	5663	1334	0.228
7	12.413	14602	2161	0.588
8	12.546	3738	633	0.151
9	12.784	930	167	0.037
10	18.212	8490	1475	0.342
Total		2481263	426011	100.000