

Sample Name :[Arg8]-Vasopressin (AVP)
 Cat No. :RP20275
 Lot No. :E9322421C
 Time Processed :4:58:21
 Month-Day-Year Processed :03/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

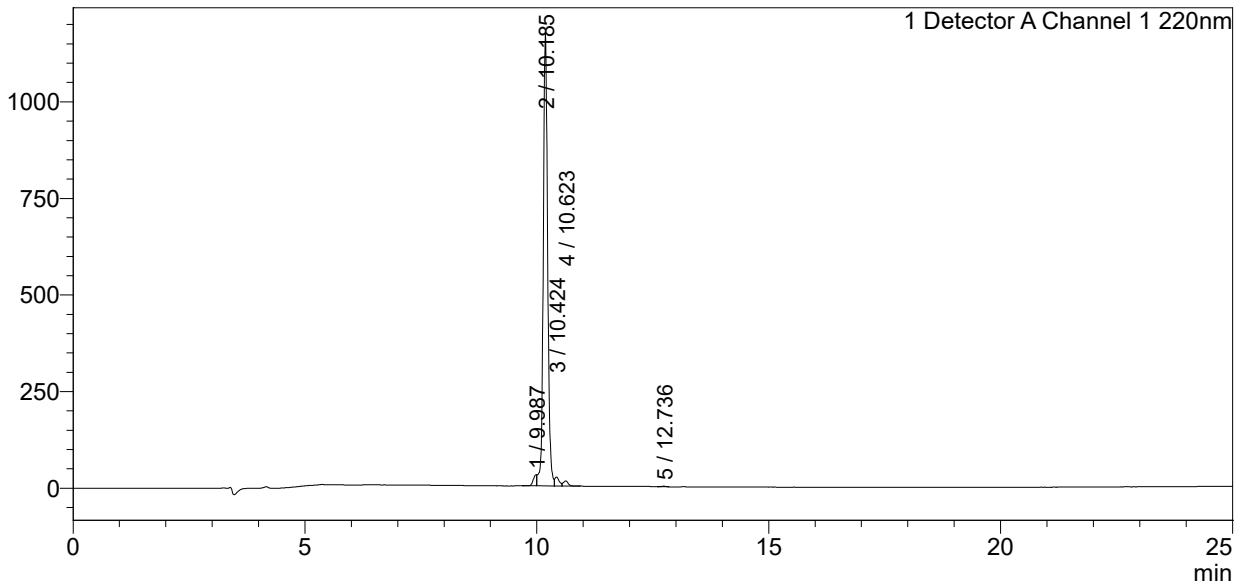

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.987	148517	28247	1.828
2	10.185	7716503	1170620	95.002
3	10.424	153984	23270	1.896
4	10.623	94761	13358	1.167
5	12.736	8669	1606	0.107
Total		8122433	1237101	100.000