

Sample Name : TP508
 Cat. No. : RP20095
 Lot. No. : E7029619J
 Time Processed : 15:07:48
 Month-Day-Year Processed : 10/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	20	
25.00	Pumps	Pump A B.Conc	80	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	20	
40.00	Pumps	Pump A B.Conc	20	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

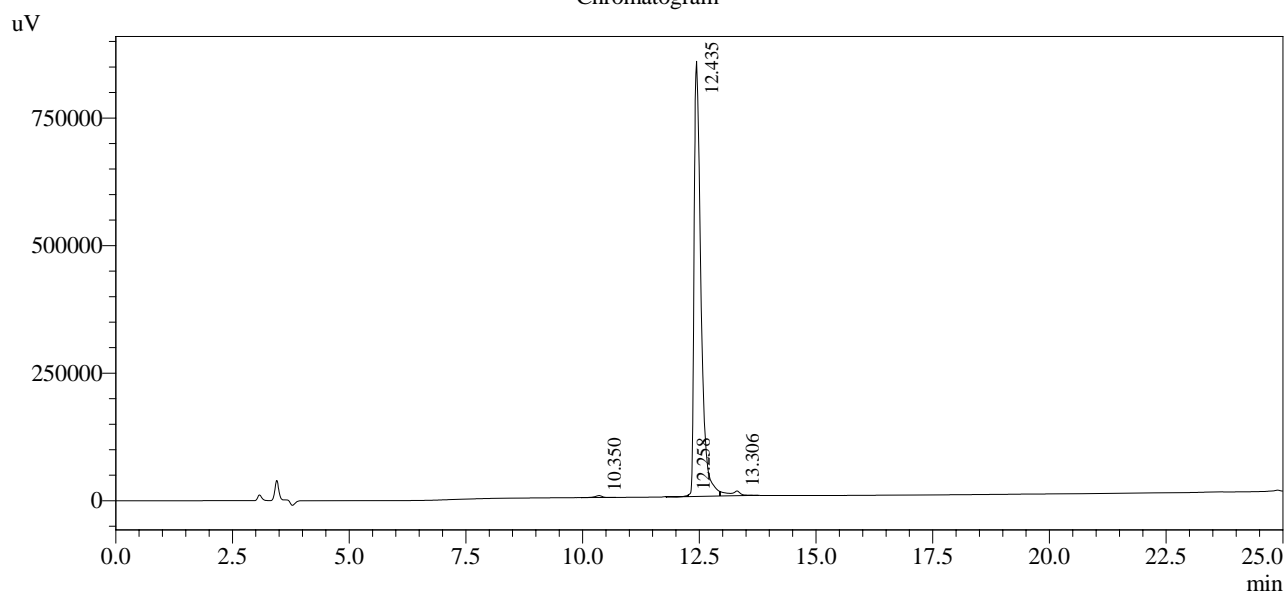

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.350	38534	3817	0.430
2	12.258	9053	2752	0.101
3	12.435	8716378	852877	97.360
4	13.306	188783	9349	2.109
Total		8952749	868796	100.000