

Sample Name : IRL-1620  
 Cat. No. : RP13497  
 Lot. No. : E49102191  
 Time Processed : 8:28:16  
 Month-Day-Year Processed : 10/07/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

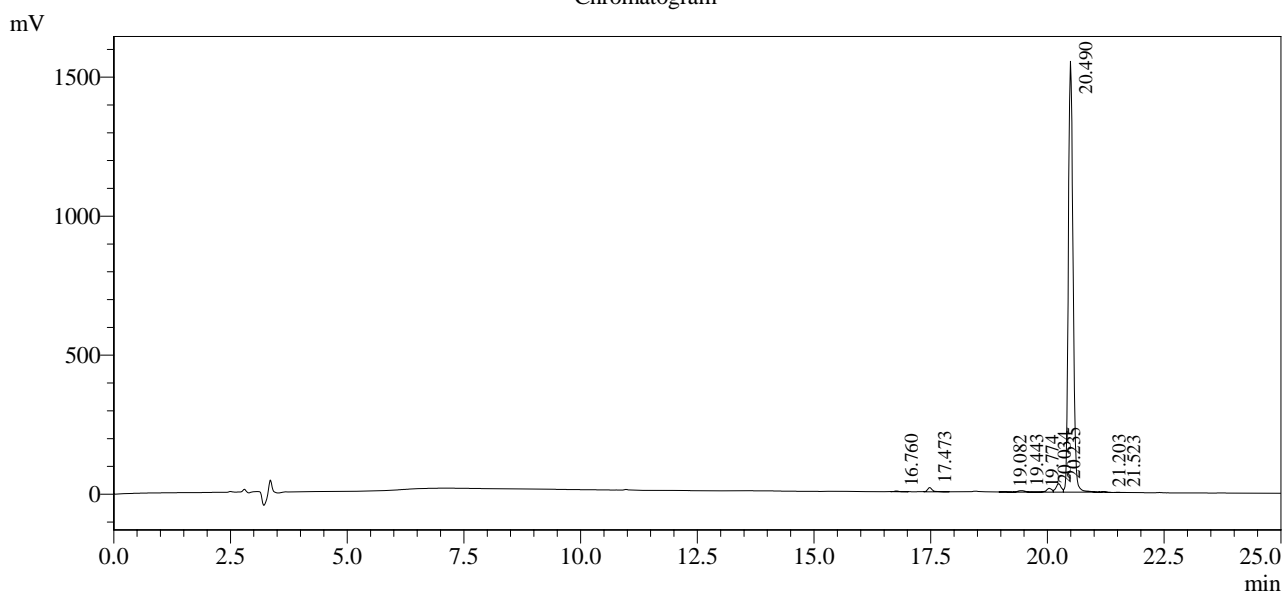

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.760	17497	2716	0.152
2	17.473	101008	14978	0.880
3	19.082	6510	735	0.057
4	19.443	55708	5085	0.485
5	19.774	5093	627	0.044
6	20.034	108977	13656	0.950
7	20.235	236007	30323	2.057
8	20.490	10924257	1549762	95.205
9	21.203	16218	2527	0.141
10	21.523	3154	428	0.027
Total		11474429	1620837	100.000