

Sample Name : Calcitonin, eel
Cat No.: RP12786
Lot No.: E7023619J
Time Processed : 1:08:44
Month-Day-Year Processed : 10/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow: 1 ml/min
Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	20
25.00	Pumps	Pump A B.Conc	80
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	20
40.00	Pumps	Pump A B.Conc	20
40.10	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ19010324

<Chromatogram>

mV

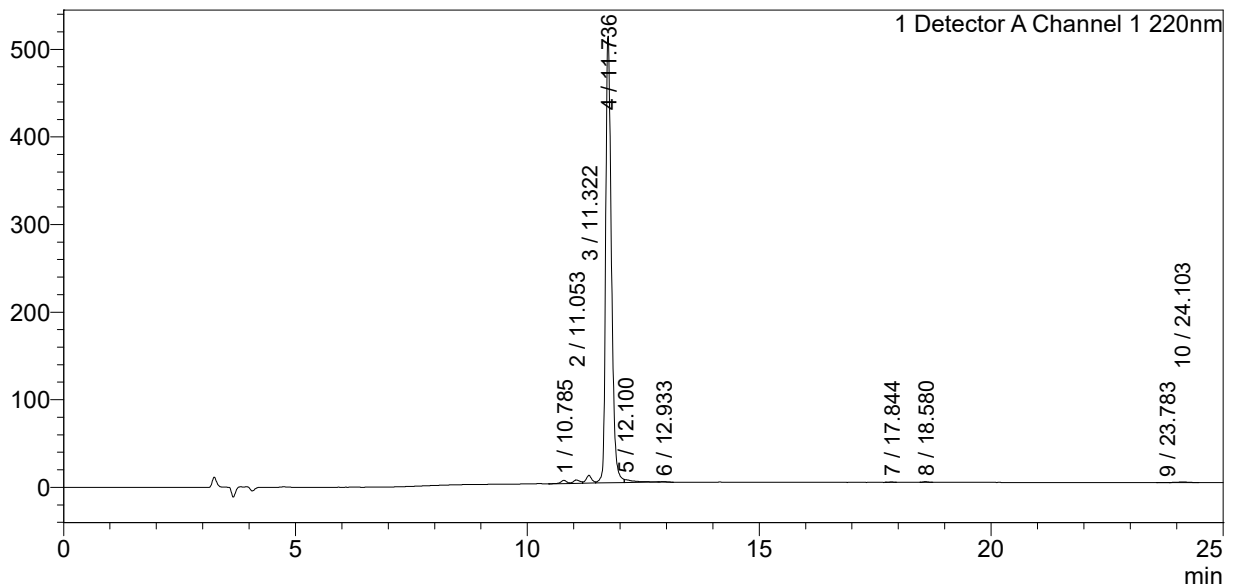

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.785	32187	3666	0.696
2	11.053	38449	3940	0.831
3	11.322	75263	8973	1.627
4	11.736	4406948	510288	95.260
5	12.100	48624	3401	1.051
6	12.933	4451	566	0.096
7	17.844	2447	443	0.053
8	18.580	5249	871	0.113
9	23.783	940	98	0.020
10	24.103	11677	602	0.252
Total		4626234	532848	100.000