


Mass Spectrum

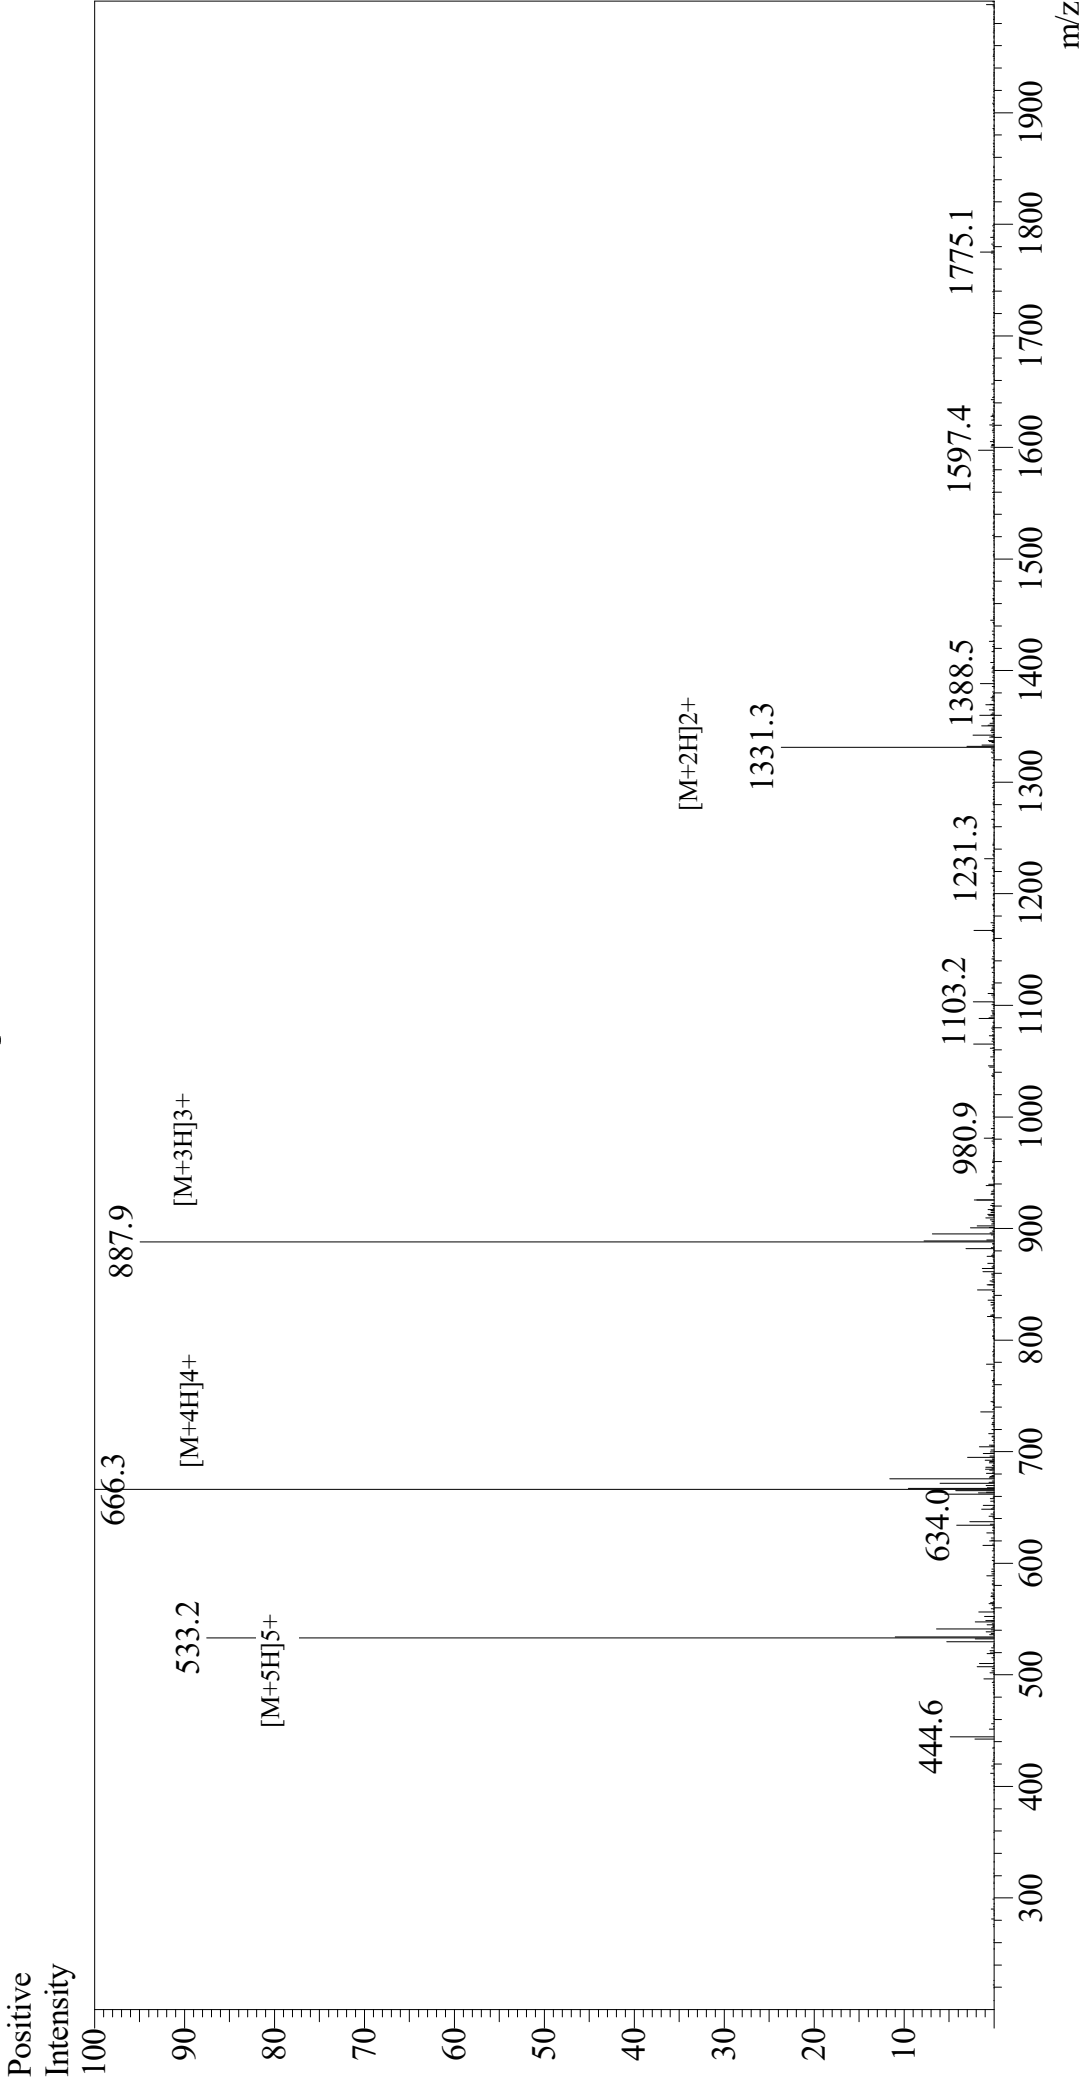

Sample Information

Acquired by : Gary
 Month-Day Processed : 12/09/18
 Time Processed : 09:44:05 AM
 Injection Volume : 0.2
 Sample Name : β -Melanocyte Stimulating Hormone (MSH), human
 Cat No. : RP10648
 Lot No. : PE3801812
 Theoretical MW : 2661.00
 Observed MW : 2661.2

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H2O/50% MeOH