

Sample Name :Syntide 2  
 Cat No. :RP10322  
 Lot No. :E5985220C  
 Time Processed :7:20:12  
 Month-Day-Year Processed :03/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command         | Value |
|-------|------------|-----------------|-------|
| 0.01  | Pumps      | Solvent B Conc. | 5     |
| 25.00 | Pumps      | Solvent B Conc. | 65    |
| 25.01 | Pumps      | Solvent B Conc. | 95    |
| 27.00 | Pumps      | Solvent B Conc. | 95    |
| 27.01 | Pumps      | Solvent B Conc. | 5     |
| 33.00 | Pumps      | Solvent B Conc. | 5     |
| 33.01 | Controller | Stop            |       |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

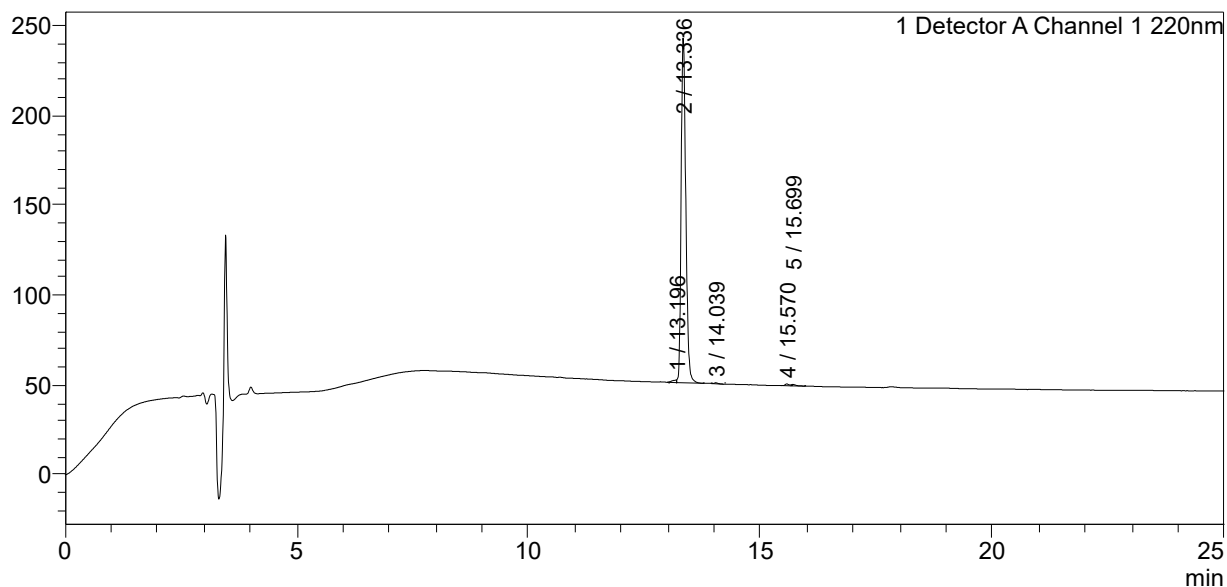

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area    | Height | Area%   |
|-------|-----------|---------|--------|---------|
| 1     | 13.196    | 9905    | 1481   | 0.726   |
| 2     | 13.336    | 1340083 | 191832 | 98.205  |
| 3     | 14.039    | 2550    | 518    | 0.187   |
| 4     | 15.570    | 5867    | 1011   | 0.430   |
| 5     | 15.699    | 6169    | 838    | 0.452   |
| Total |           | 1364574 | 195681 | 100.000 |