

Sample Name :PA (224-233), Influenza
 Cat No:RP19991
 Lot No :E5634220K
 Time Processed :4:20:49 AM
 Month-Day-Year Processed :11/22/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

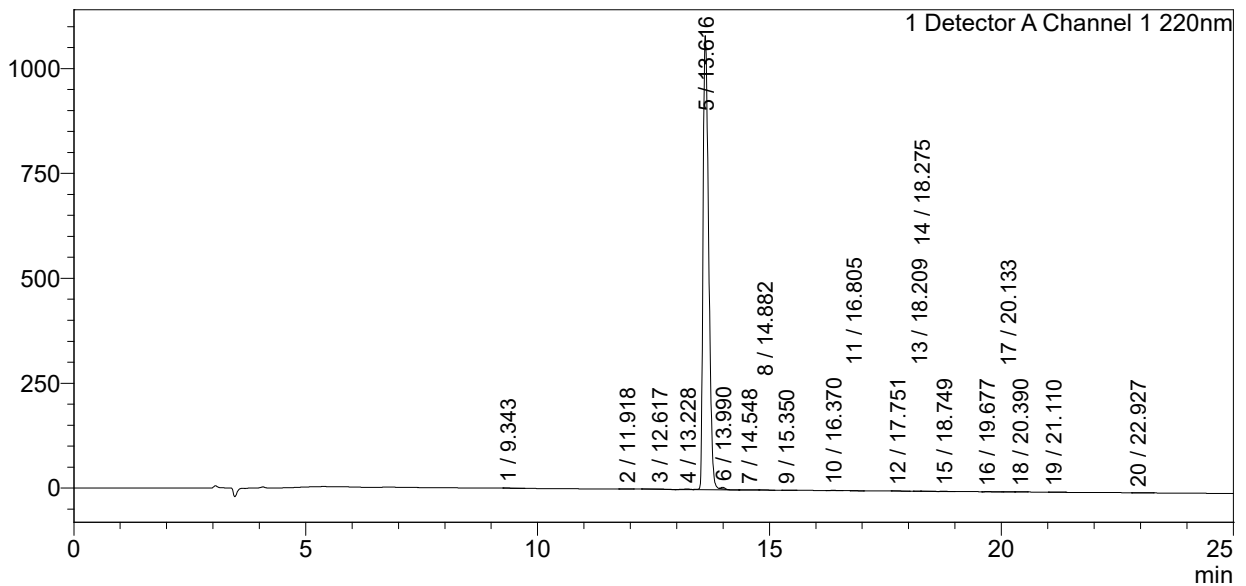

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.343	1987	174	0.022
2	11.918	1342	118	0.015
3	12.617	19411	1042	0.212
4	13.228	15956	1544	0.174
5	13.616	9072643	1082649	98.912
6	13.990	20770	3934	0.226
7	14.548	4566	400	0.050
8	14.882	4797	732	0.052
9	15.350	1308	120	0.014
10	16.370	7059	897	0.077
11	16.805	1528	129	0.017
12	17.751	2126	167	0.023
13	18.209	1224	199	0.013
14	18.275	2948	233	0.032
15	18.749	1838	163	0.020
16	19.677	4149	203	0.045

Peak#	Ret. Time	Area	Height	Area%
17	20.133	1021	125	0.011
18	20.390	2227	266	0.024
19	21.110	2599	197	0.028
20	22.927	2933	197	0.032
Total		9172433	1093491	100.000