


Mass Spectrum

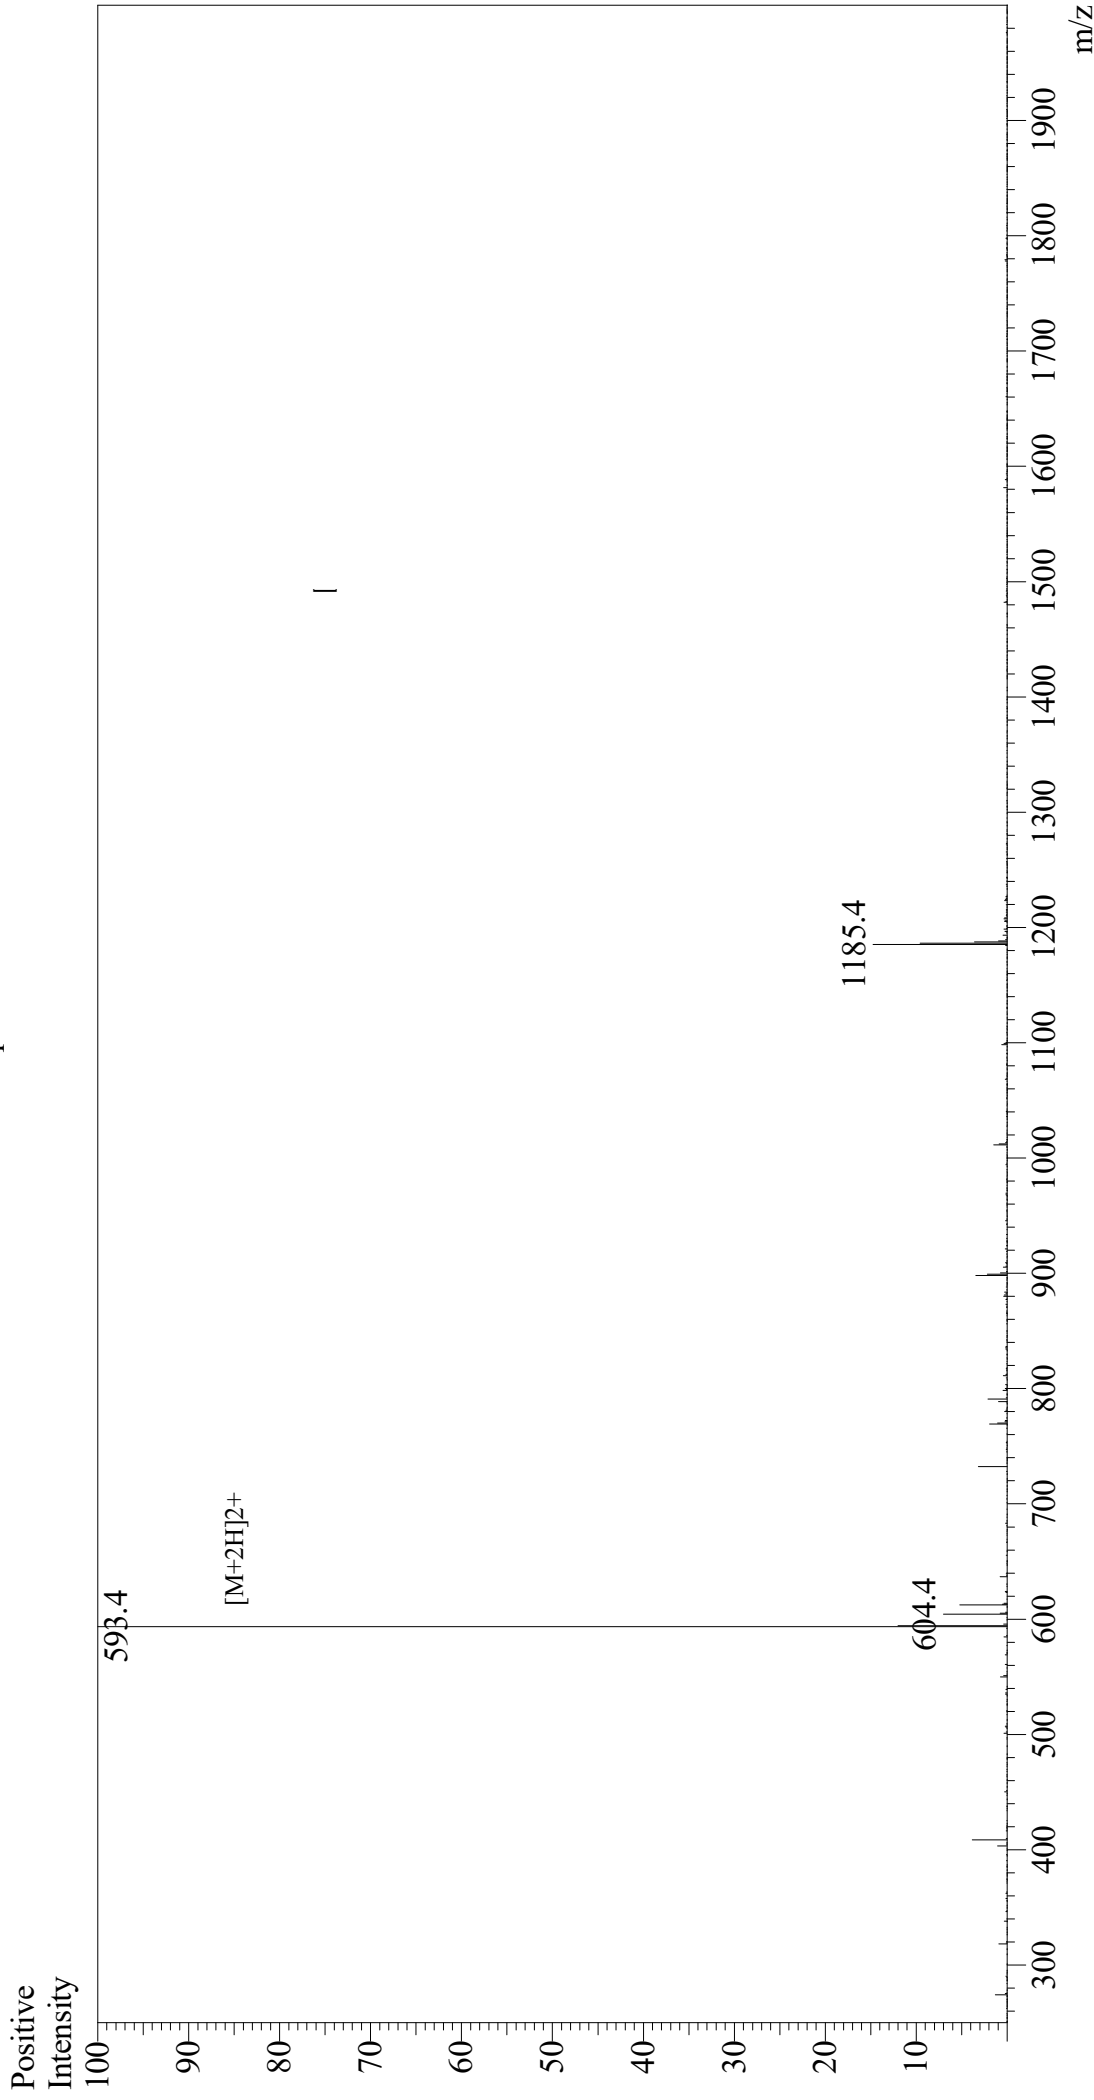

Sample Information
Month-Day Processed : 11/22/20
Time Processed : 09:23:50 AM
Injection Volume : 0.4
Sample Name : PA (224-233), Influenza
Cat No. : RP19991
Lot No. : E5634220K
Theoretical MW : 1185.29
Observed MW : 1184.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH